

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072018\
 Data File : BF107574.D
 Acq On : 21 Jul 2018 14:14
 Operator : JU/SJ
 Sample : J4094-07
 Misc :
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 071818-TIPC-E-D-M

Quant Time: Jul 23 05:01:40 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 20 16:29:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	345801	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	1270649	20.00	ng	0.00
38) Acenaphthene-d10	10.02	164	487576	20.00	ng	0.00
63) Phenanthrene-d10	11.51	188	824267	20.00	ng	0.00
75) Chrysene-d12	14.16	240	752596	20.00	ng	0.00
86) Perylene-d12	15.69	264	587716	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.60	112	784193	36.46	ng	0.00
7) Phenol-d6	6.60	99	703428	27.24	ng	-0.02
23) Nitrobenzene-d5	7.54	82	1800049	95.61	ng	-0.01
41) 2,4,6-Tribromophenol	10.81	330	430105	77.57	ng	0.00
44) 2-Fluorobiphenyl	9.33	172	2853149	107.69	ng	0.00
78) Terphenyl-d14	13.09	244	2137308	72.70	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072018\
Data File : BF107574.D
Acq On : 21 Jul 2018 14:14
Operator : JU/SJ
Sample : J4094-07
Misc :
ALS Vial : 46 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
071818-TIPC-E-D-M

Quant Time: Jul 23 05:01:40 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

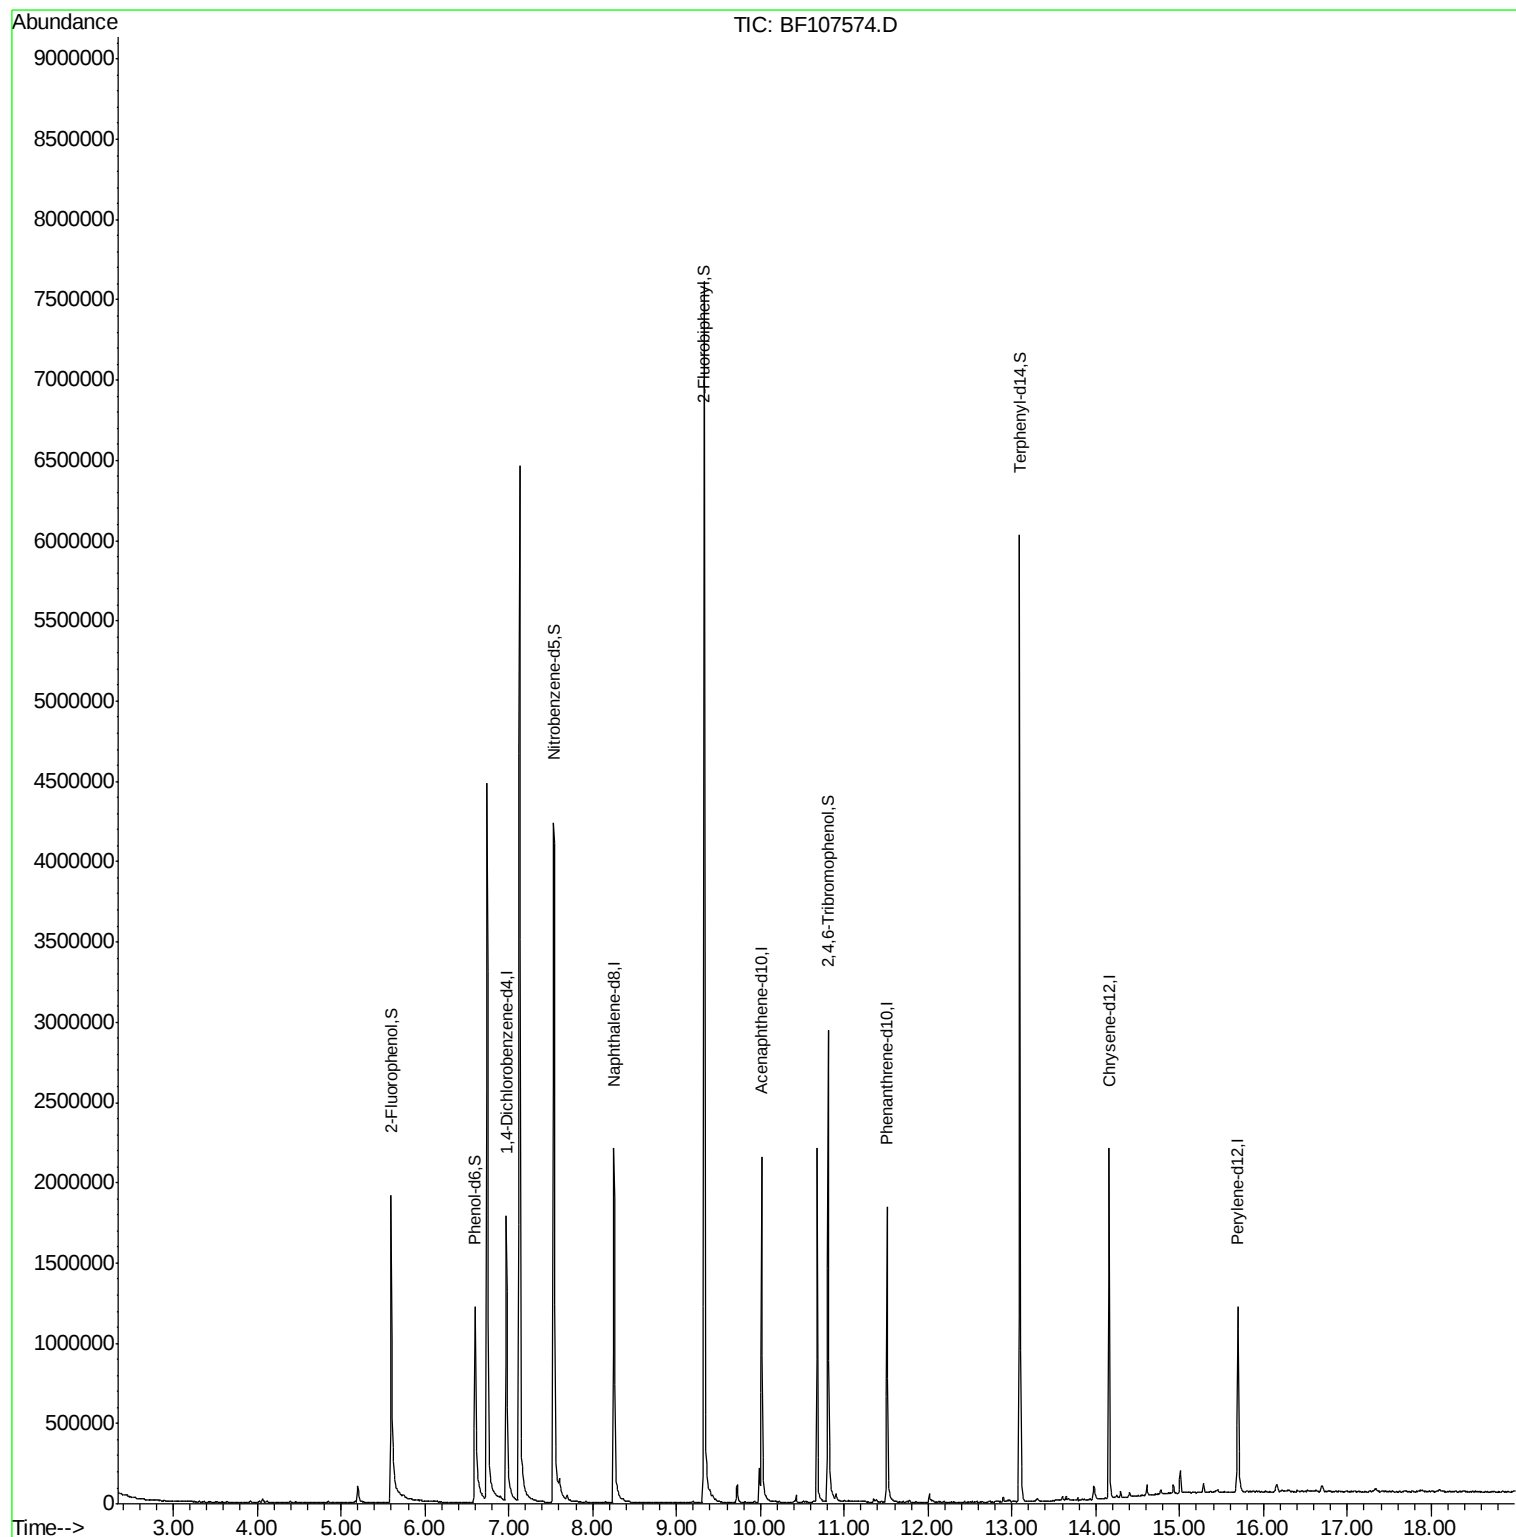

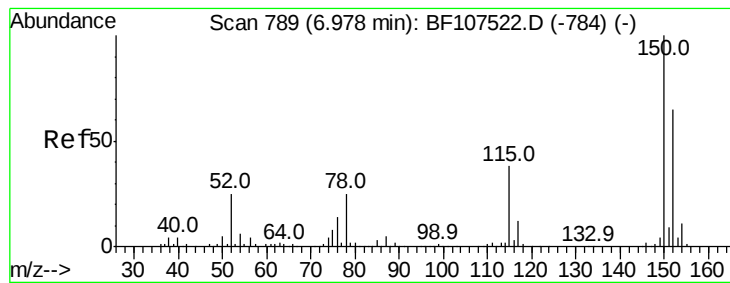


#1




1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 6.97 min Scan# 788
Delta R.T. -0.01 min
Lab File: BF107574.D
Acq: 21 Jul 2018 14:14

Instrument :
BNA_F
ClientSampleId :
071818-TIPC-E-D-M

Tot Ion	Ratio	Lower	Upper
152	100		
150	154.1	124.6	186.8
115	58.8	50.1	75.1

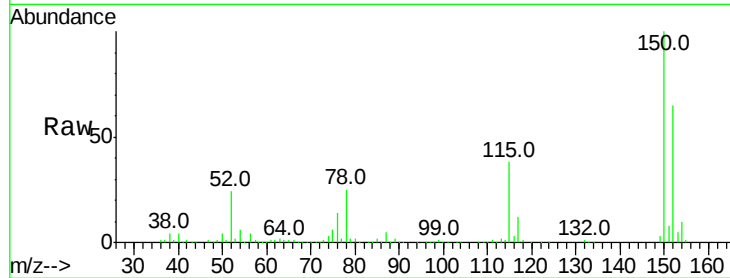


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

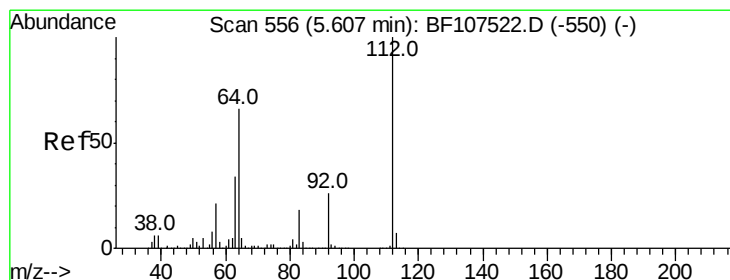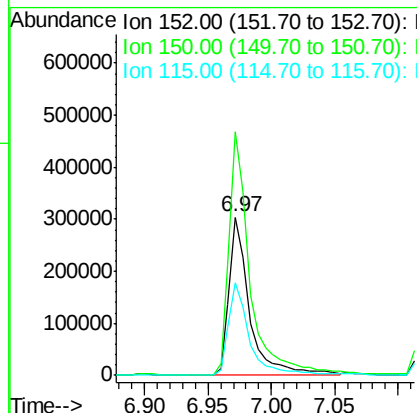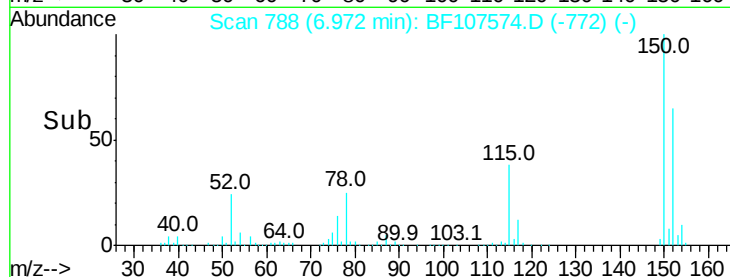



#5


2-Fluorophenol
Concen: 36.461 ng
RT: 5.60 min Scan# 555
Delta R.T. -0.01 min
Lab File: BF107574.D
Acq: 21 Jul 2018 14:14

Tgt Ion	Ratio	Lower	Upper
112	100		
64	61.6	47.9	71.9
63	32.5	23.7	35.5

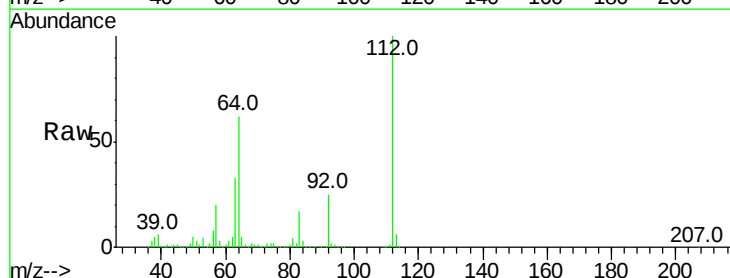

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BF1
Ion 63.00 (62.70 to 63.70): BF1

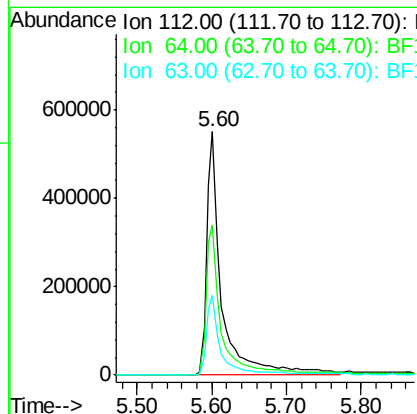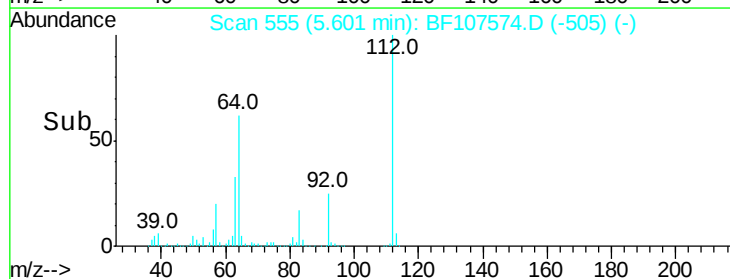

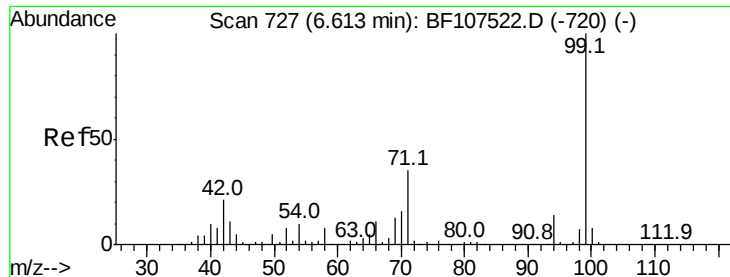

#7

Phenol-d6

Concen: 27.238 ng

RT: 6.60 min Scan# 724

Delta R.T. -0.02 min

Lab File: BF107574.D

Acq: 21 Jul 2018 14:14

Instrument :

BNA_F

ClientSampleId :

071818-TIPC-E-D-M


Tot Ion: 99 Resp: 703428

Ion Ratio Lower Upper




99 100

42 19.8 14.5 21.7

71 33.2 25.4 38.0

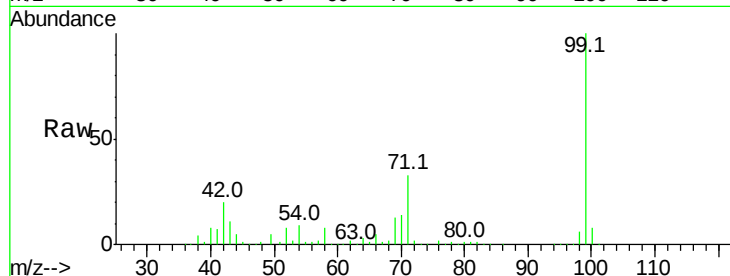

Abundance Ion 99.00 (98.70 to 99.70): BF1
Ion 42.00 (41.70 to 42.70): BF1
Ion 71.00 (70.70 to 71.70): BF1

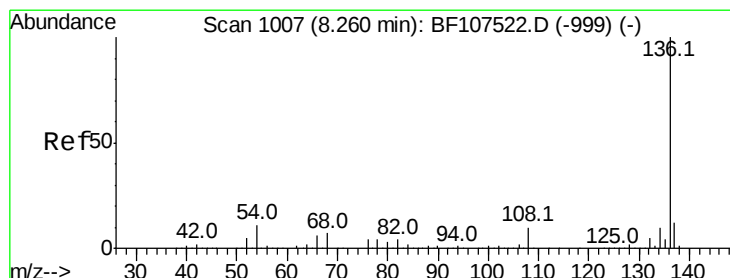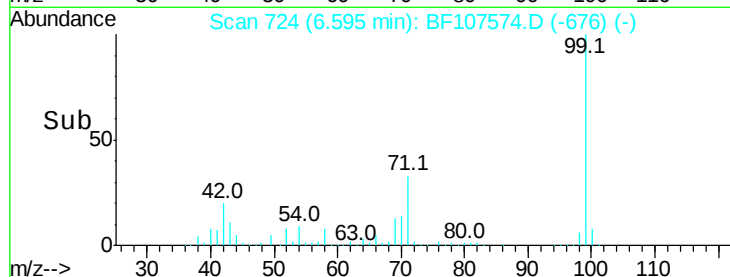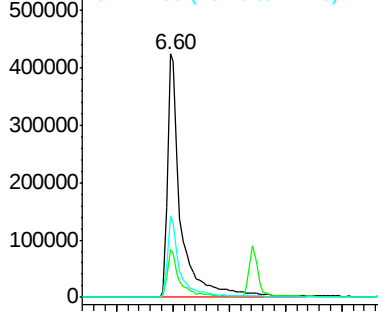

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1006

Delta R.T. -0.01 min

Lab File: BF107574.D

Acq: 21 Jul 2018 14:14

Tgt Ion: 136 Resp: 1270649


Ion Ratio Lower Upper

136 100



137 11.7 8.9 13.3


54 10.6 6.6 9.8#

68 6.9 5.0 7.4

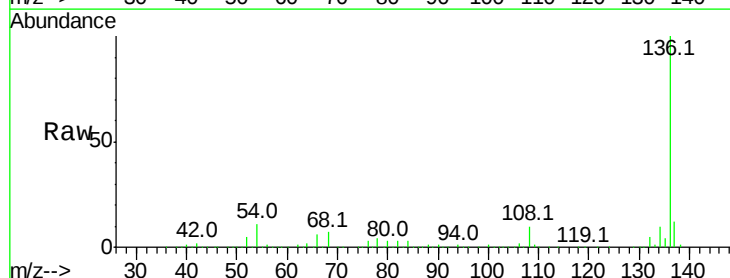

Abundance Ion 136.00 (135.70 to 136.70): E
Ion 137.00 (136.70 to 137.70): E
Ion 54.00 (53.70 to 54.70): BF1
Ion 68.00 (67.70 to 68.70): BF1

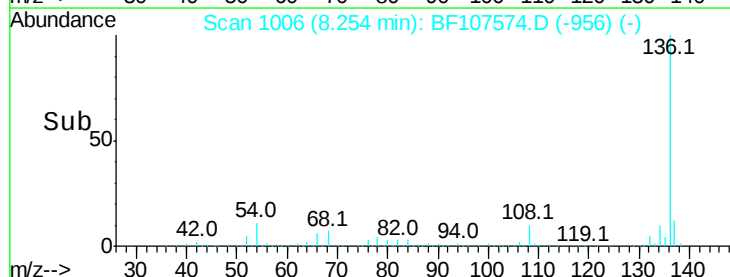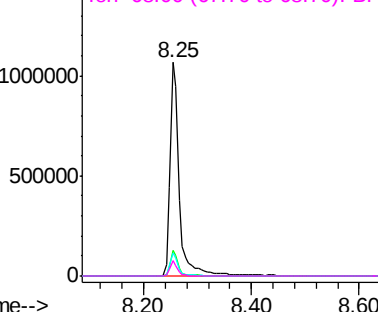


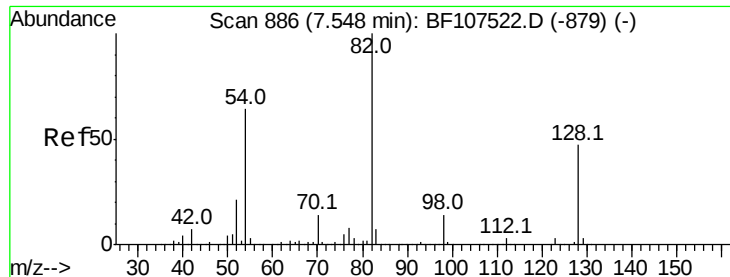




#23
 Nitrobenzene-d5
 Concen: 95.606 ng
 RT: 7.54 min Scan# 884
 Delta R.T. -0.01 min
 Lab File: BF107574.D
 Acq: 21 Jul 2018 14:14

Instrument :
 BNA_F
 ClientSampleId :
 071818-TIPC-E-D-M

Tot Ion: 82 Resp: 1800049
 Ion Ratio Lower Upper
 82 100
 128 46.1 36.1 54.1
 54 63.8 41.4 62.2#

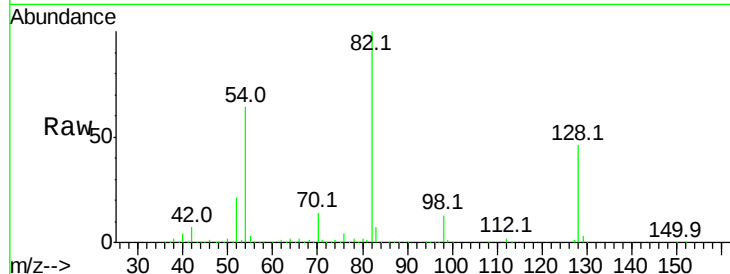


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): BF1
 Ion 54.00 (53.70 to 54.70): BF1

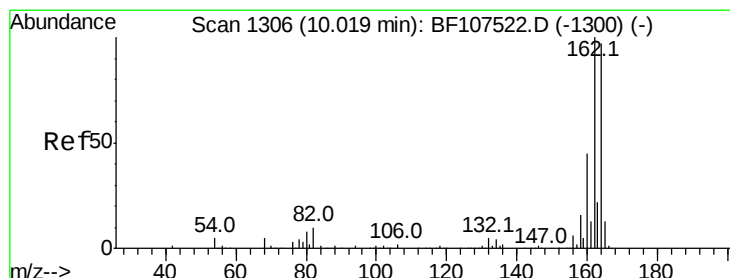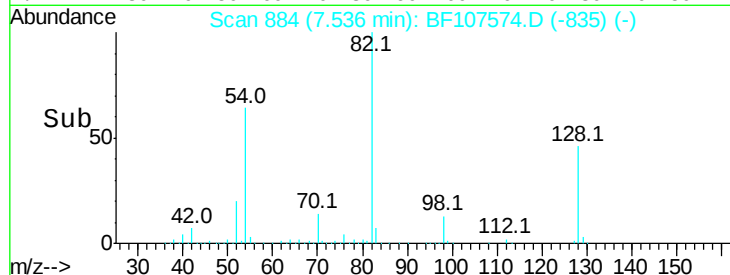
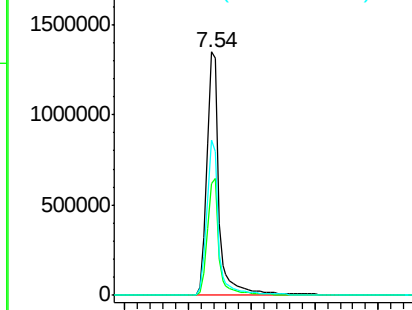



#38
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 10.02 min Scan# 1306
 Delta R.T. -0.00 min
 Lab File: BF107574.D
 Acq: 21 Jul 2018 14:14

Tgt Ion:164 Resp: 487576
 Ion Ratio Lower Upper
 164 100
 162 105.3 86.1 129.1
 160 49.7 38.3 57.5

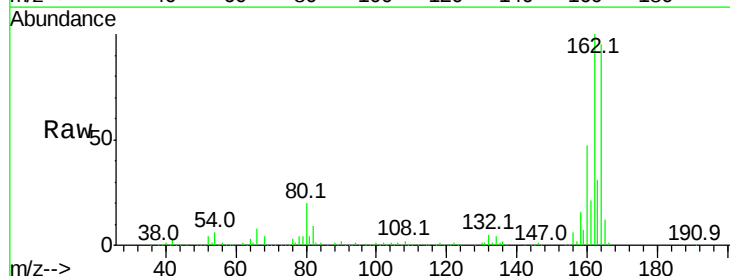

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

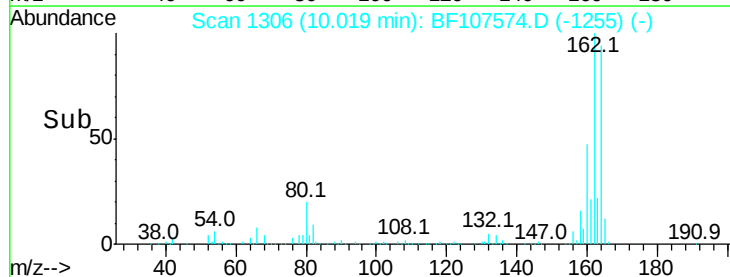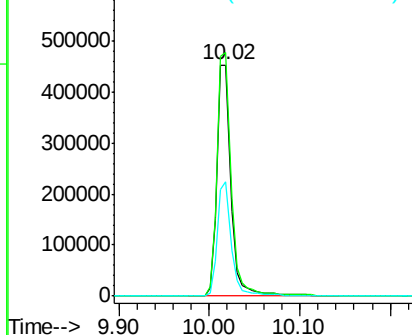


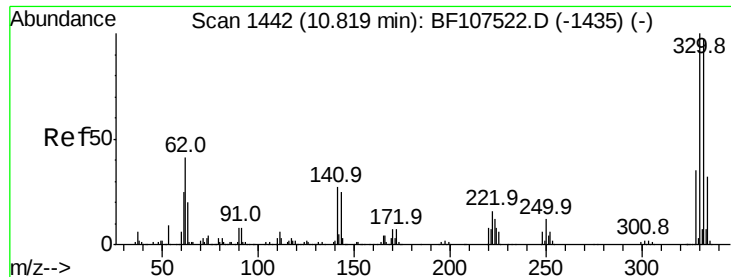




#41
 2,4,6-Tribromophenol
 Concen: 77.573 ng
 RT: 10.81 min Scan# 1441
 Delta R.T. -0.01 min
 Lab File: BF107574.D
 Acq: 21 Jul 2018 14:14

Instrument :
 BNA_F
 ClientSampleId :
 071818-TIPC-E-D-M

Tot Ion:330 Resp: 430105
 Ion Ratio Lower Upper
 330 100
 332 96.9 77.0 115.6
 141 30.5 29.9 44.9

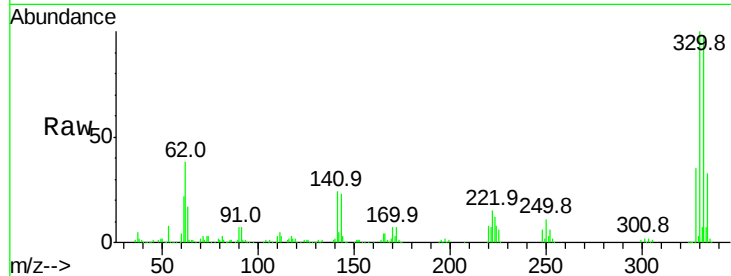


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

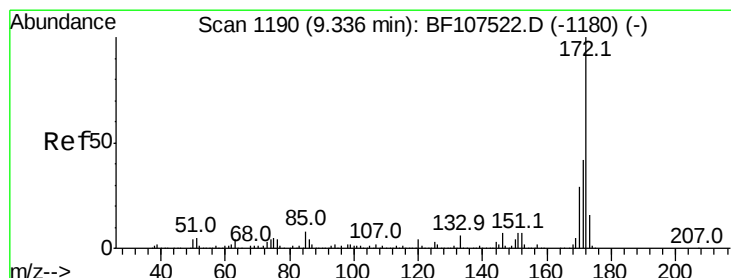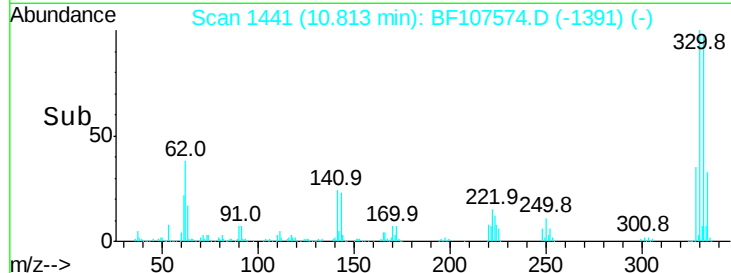
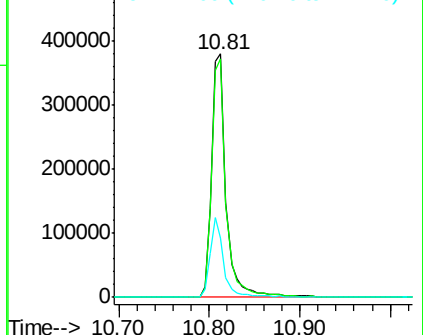



#44
 2-Fluorobiphenyl
 Concen: 107.693 ng
 RT: 9.33 min Scan# 1189
 Delta R.T. -0.01 min
 Lab File: BF107574.D
 Acq: 21 Jul 2018 14:14

Tgt Ion:172 Resp: 2853149
 Ion Ratio Lower Upper
 172 100
 171 39.9 29.7 44.5
 170 27.4 19.6 29.4

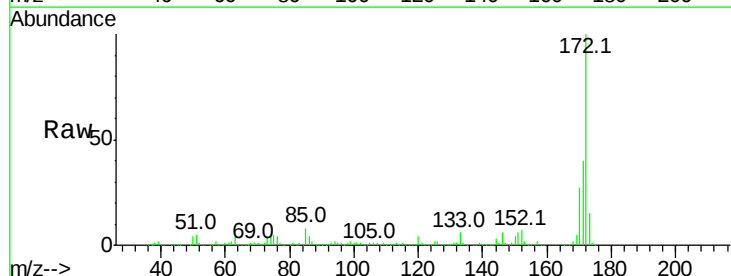

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E



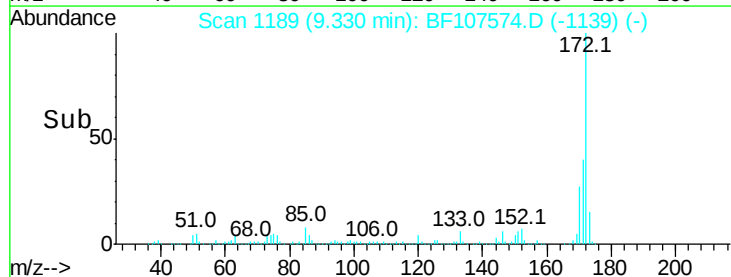
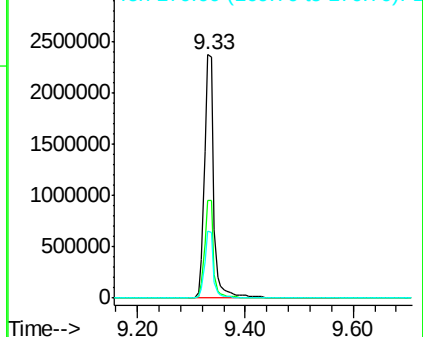


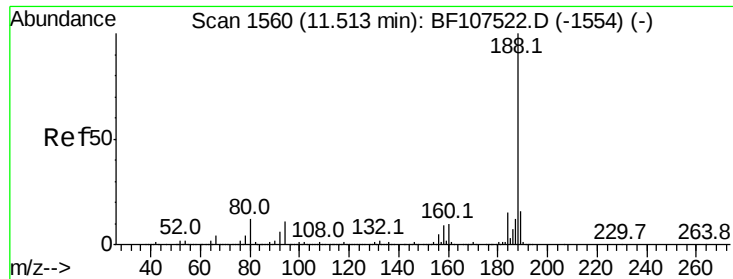

#63
Phenanthrene-d10
Concen: 20.000 ng
RT: 11.51 min Scan# 1560
Delta R.T. -0.00 min
Lab File: BF107574.D
Acq: 21 Jul 2018 14:14




Instrument :
BNA_F
ClientSampleId :
071818-TIPC-E-D-M


Tot Ion:188 Resp: 824267
Ion Ratio Lower Upper
188 100
94 9.4 8.5 12.7
80 9.9 9.2 13.8

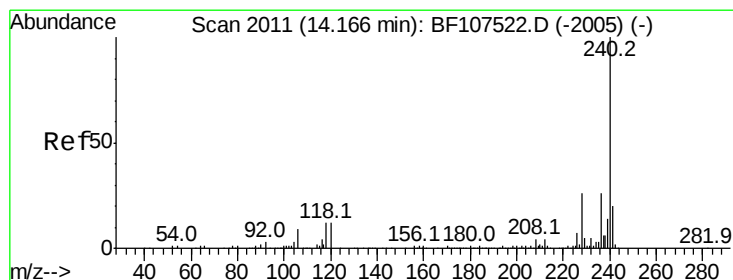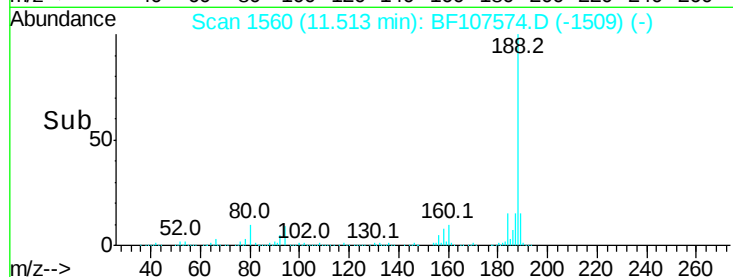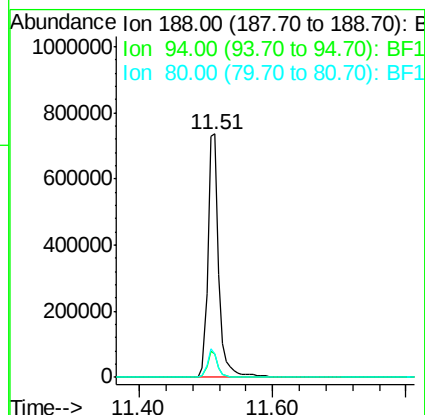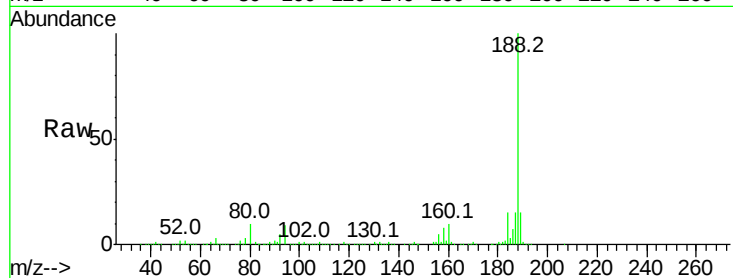

#75
Chrysene-d12
Concen: 20.000 ng
RT: 14.16 min Scan# 2010
Delta R.T. -0.01 min
Lab File: BF107574.D
Acq: 21 Jul 2018 14:14

Tgt Ion:240 Resp: 752596
Ion Ratio Lower Upper
240 100
120 12.7 9.5 14.3
236 25.8 20.7 31.1

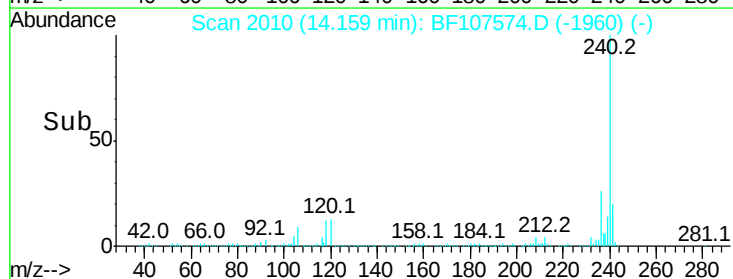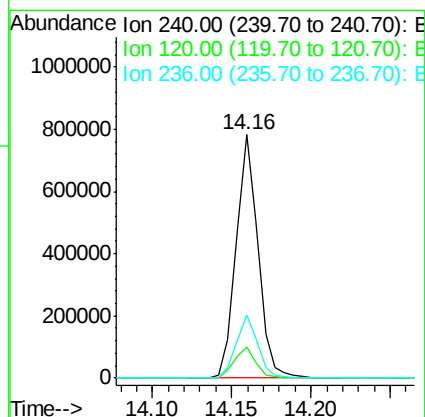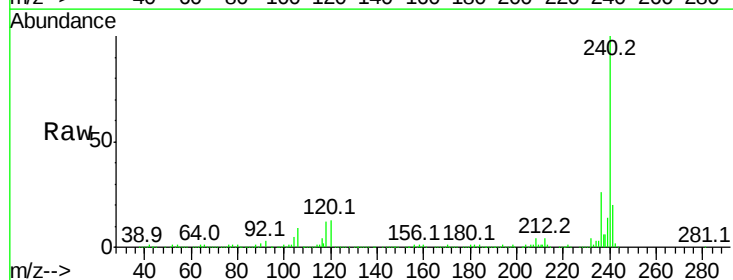

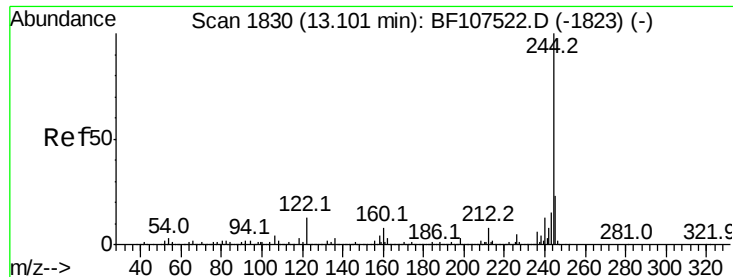

#78

Terphenyl-d14

Concen: 72.704 ng

RT: 13.09 min Scan# 1829

Delta R.T. -0.01 min

Lab File: BF107574.D

Acq: 21 Jul 2018 14:14

Instrument :


BNA_F

ClientSampleId :

071818-TIPC-E-D-M

Tot Ion:244 Resp: 2137308




Ion	Ratio	Lower	Upper
244	100		
212	7.7	5.4	8.0
122	13.0	11.0	16.4

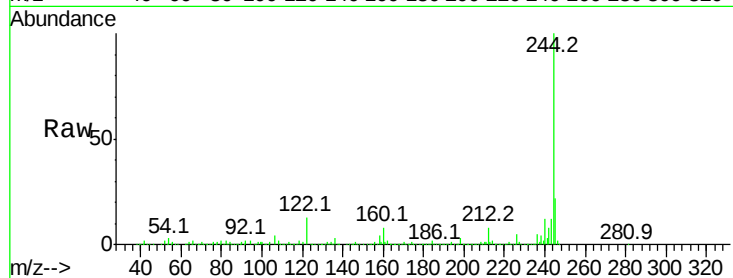

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

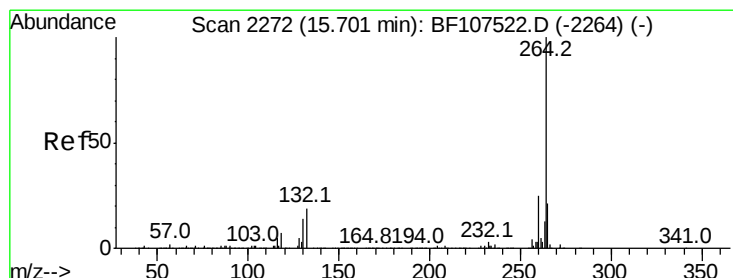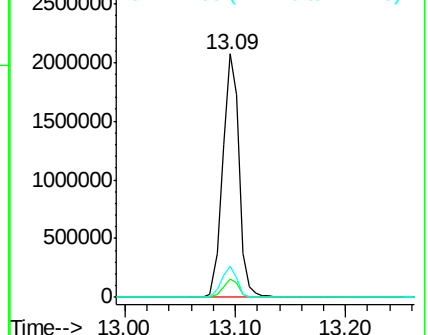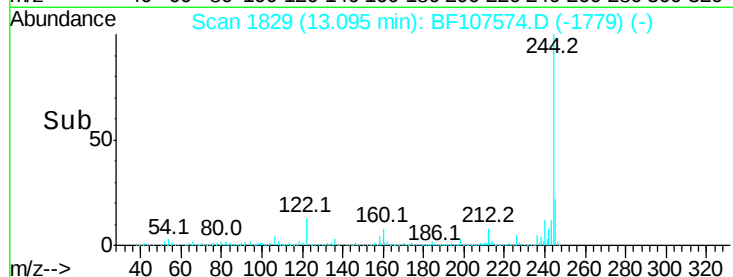

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.69 min Scan# 2271


Delta R.T. -0.01 min

Lab File: BF107574.D

Acq: 21 Jul 2018 14:14

Tgt Ion:264 Resp: 587716

Ion	Ratio	Lower	Upper
264	100		
260	23.1	19.2	28.8
265	20.5	17.5	26.3

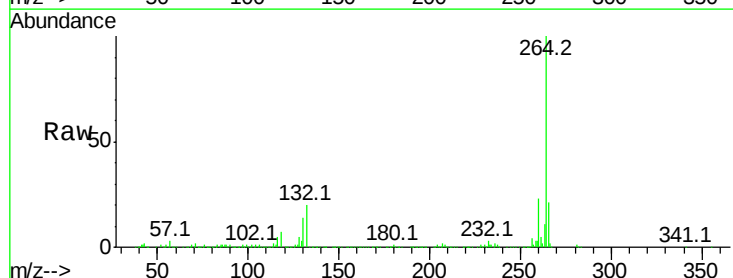

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

