

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072018\
 Data File : BF107576.D
 Acq On : 21 Jul 2018 15:08
 Operator : JU/SJ
 Sample : PB111309BL
 Misc :
 ALS Vial : 48 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB111309BL

Quant Time: Jul 23 05:07:46 2018
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 20 16:29:27 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.97	152	308111	20.00	ng	0.00
21) Naphthalene-d8	8.25	136	1151770	20.00	ng	0.00
38) Acenaphthene-d10	10.01	164	437112	20.00	ng	0.00
63) Phenanthrene-d10	11.51	188	734989	20.00	ng	0.00
75) Chrysene-d12	14.16	240	679519	20.00	ng	0.00
86) Perylene-d12	15.69	264	558706	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.61	112	1351908	70.55	ng	0.00
7) Phenol-d6	6.60	99	1656121	71.97	ng	-0.01
23) Nitrobenzene-d5	7.54	82	1455503	85.28	ng	-0.01
41) 2,4,6-Tribromophenol	10.81	330	343748	69.16	ng	-0.01
44) 2-Fluorobiphenyl	9.33	172	2463535	101.82	ng	0.00
78) Terphenyl-d14	13.09	244	1850861	69.73	ng	0.00


Target Compounds Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072018\
Data File : BF107576.D
Acq On : 21 Jul 2018 15:08
Operator : JU/SJ
Sample : PB111309BL
Misc :
ALS Vial : 48 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB111309BL

Quant Time: Jul 23 05:07:46 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

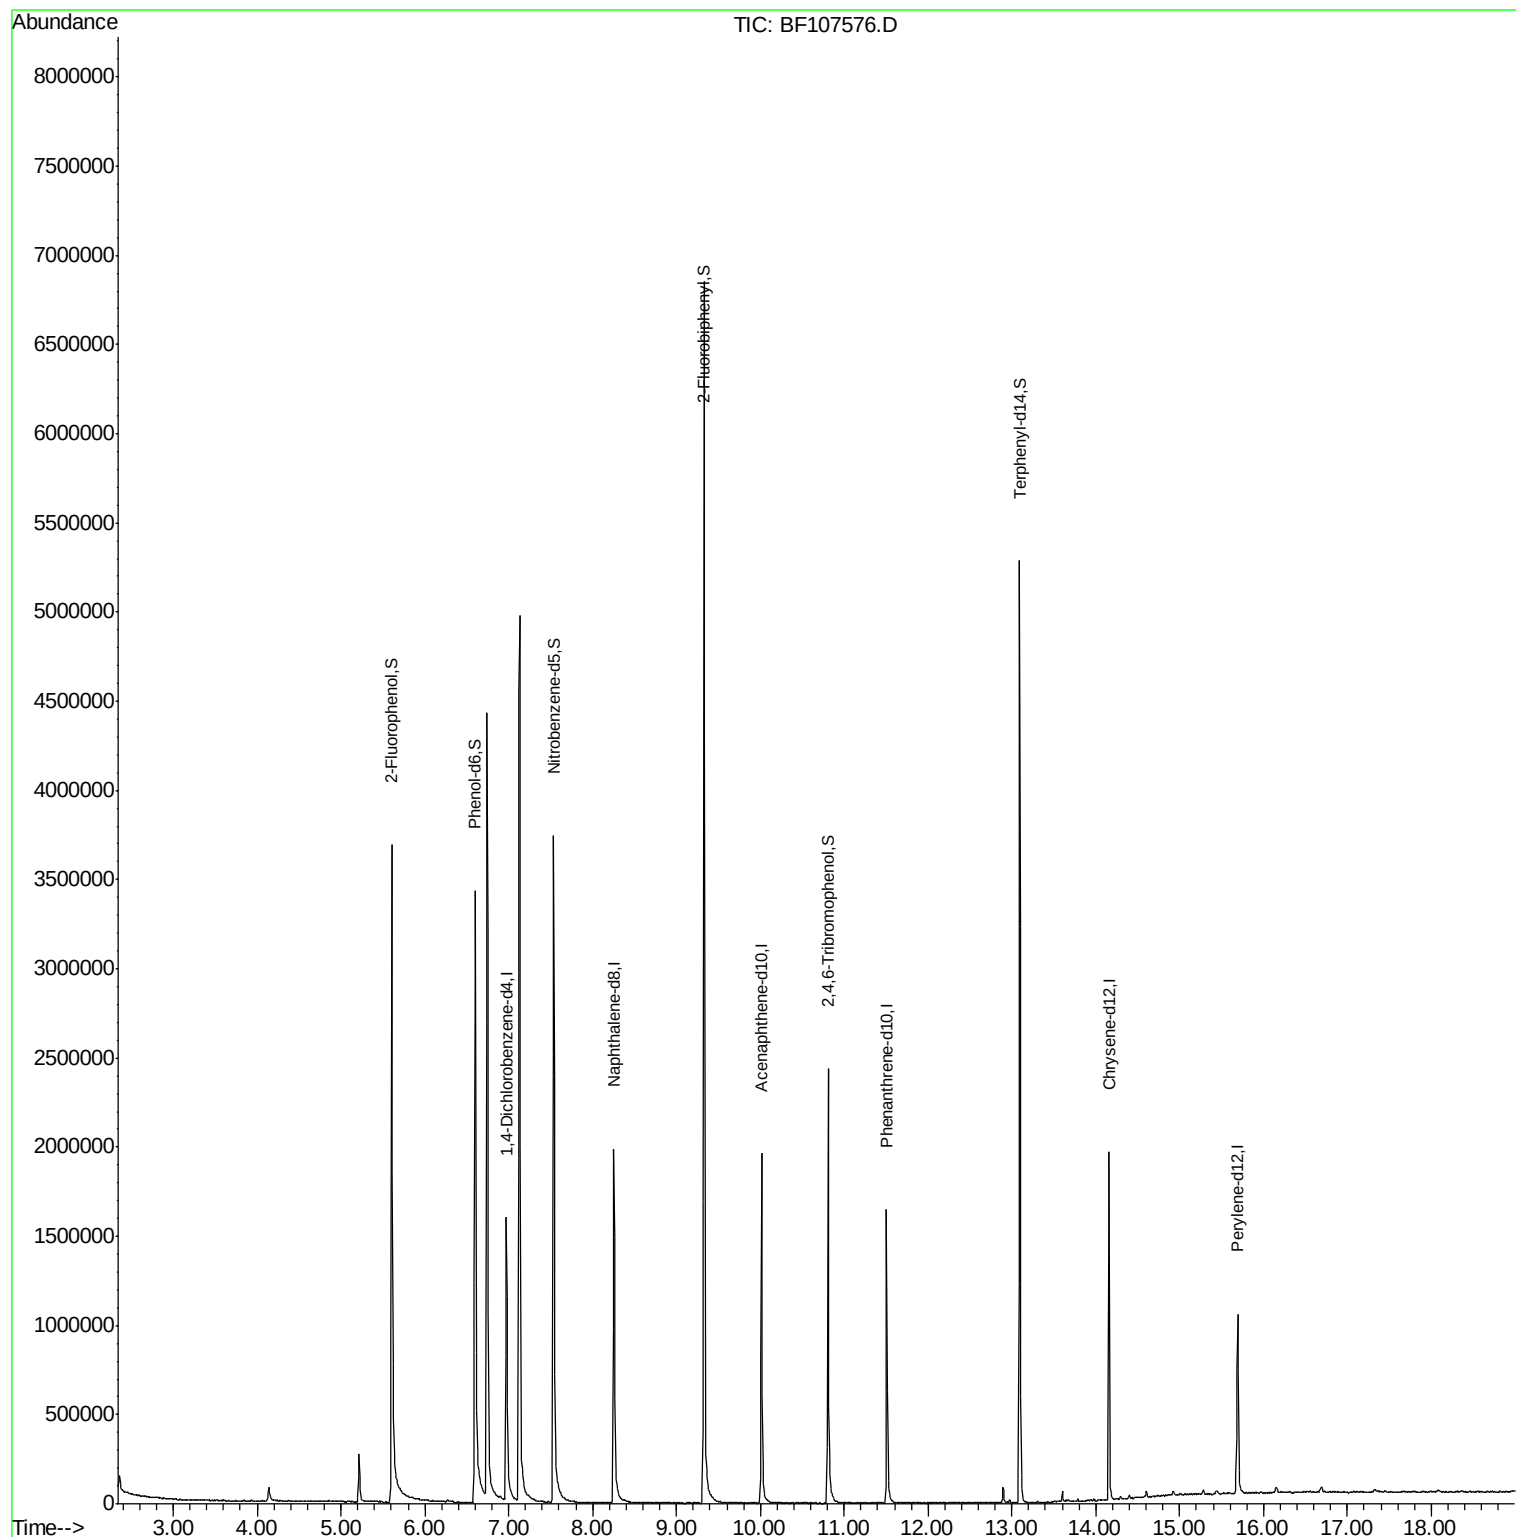




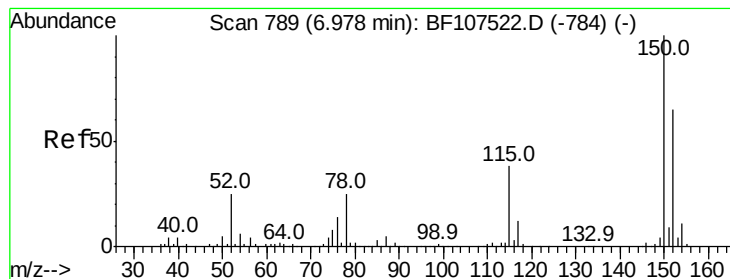


#1

1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.97 min Scan# 788
 Delta R.T. -0.01 min
 Lab File: BF107576.D
 Acq: 21 Jul 2018 15:08

Instrument :
 BNA_F
 ClientSampleId :
 PB111309BL




Tot Ion:152 Resp: 308111
 Ion Ratio Lower Upper
 152 100
 150 159.1 124.6 186.8
 115 61.4 50.1 75.1

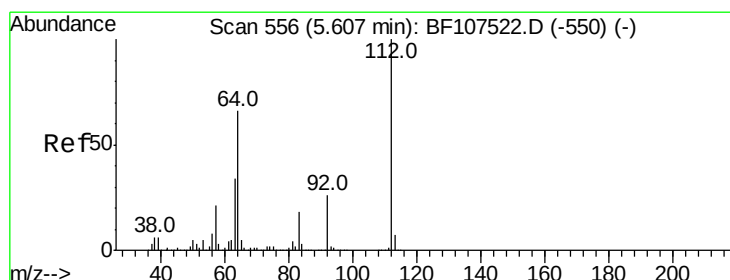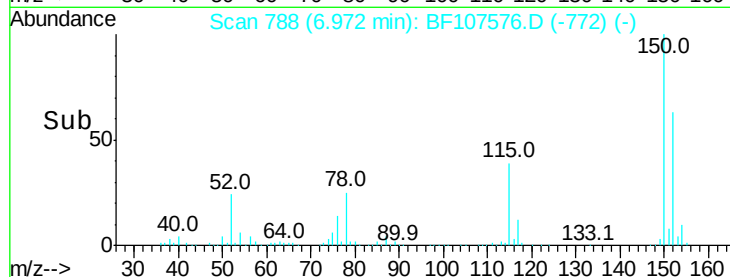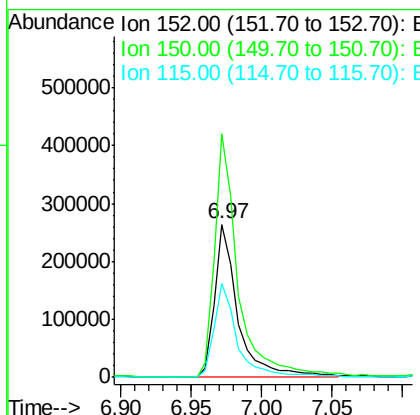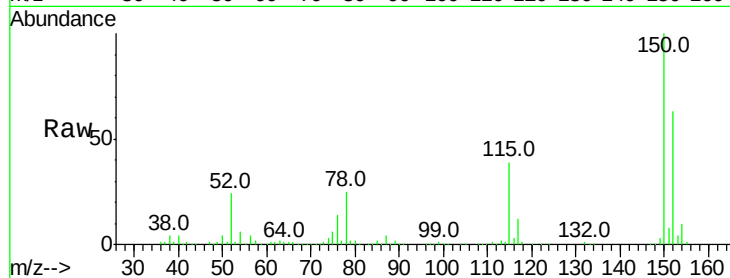


#5

2-Fluorophenol
 Concen: 70.546 ng
 RT: 5.61 min Scan# 556
 Delta R.T. 0.00 min
 Lab File: BF107576.D
 Acq: 21 Jul 2018 15:08

Tgt Ion:112 Resp: 1351908
 Ion Ratio Lower Upper
 112 100
 64 64.2 47.9 71.9
 63 32.6 23.7 35.5

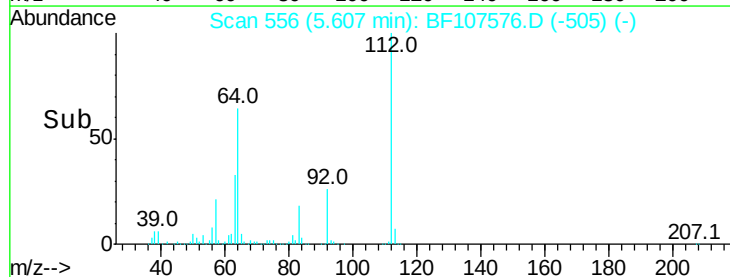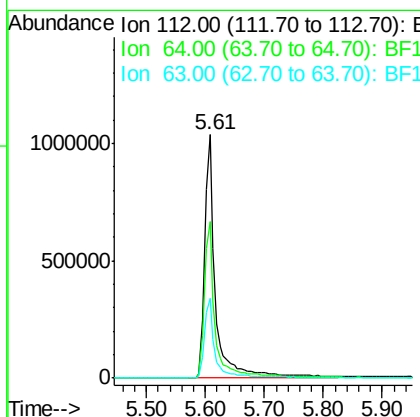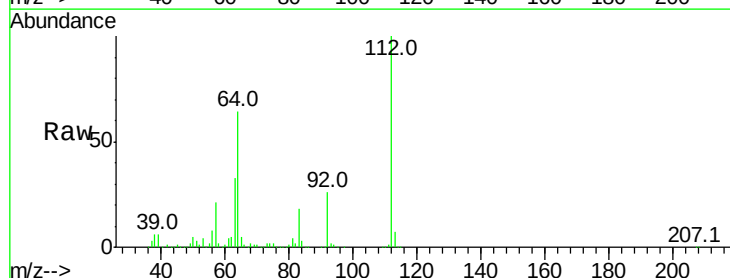

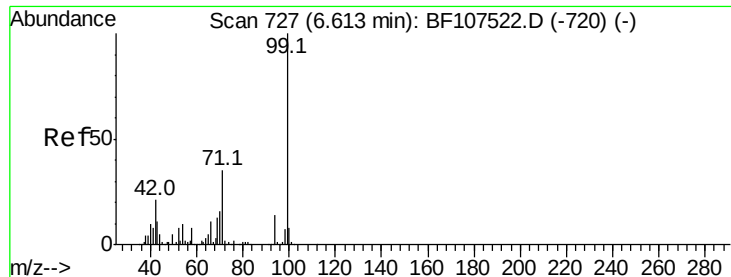

#7

Phenol-d6

Concen: 71.973 ng

RT: 6.60 min Scan# 725

Delta R.T. -0.01 min

Lab File: BF107576.D

Acq: 21 Jul 2018 15:08

Instrument :

BNA_F

ClientSampleId :

PB111309BL





Tot Ion: 99 Resp: 1656121

Ion Ratio Lower Upper

99 100

42 20.0 14.5 21.7

71 33.8 25.4 38.0

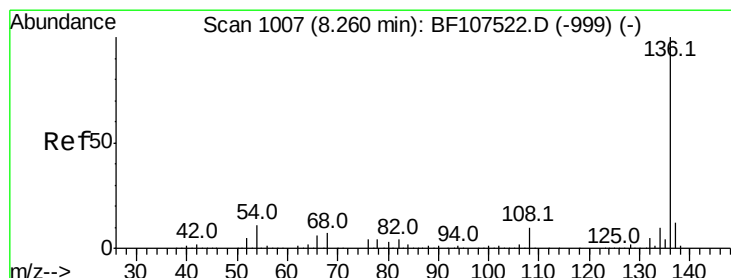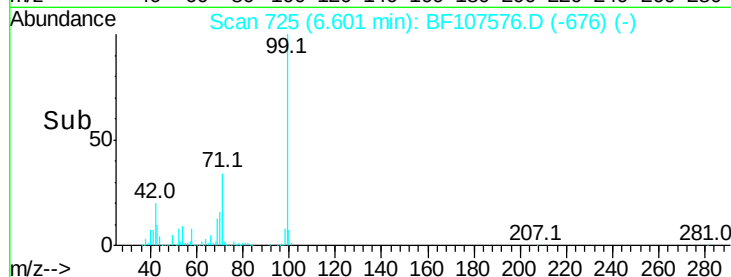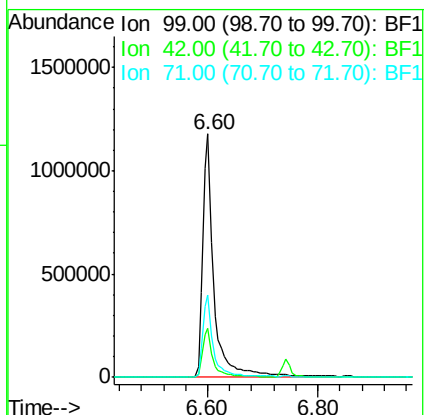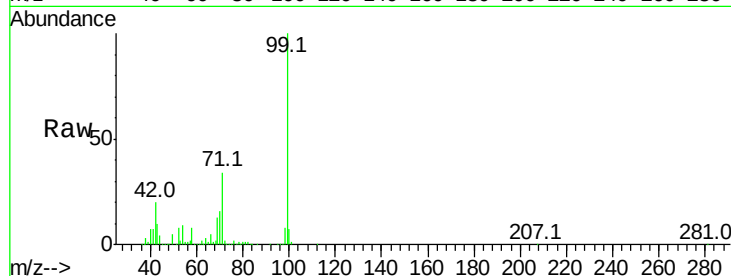

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.25 min Scan# 1006

Delta R.T. -0.01 min

Lab File: BF107576.D

Acq: 21 Jul 2018 15:08

Tgt Ion: 136 Resp: 1151770




Ion Ratio Lower Upper


136 100

137 11.5 8.9 13.3

54 10.2 6.6 9.8#

68 6.6 5.0 7.4


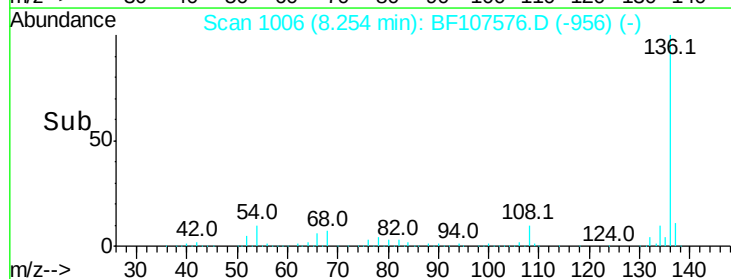
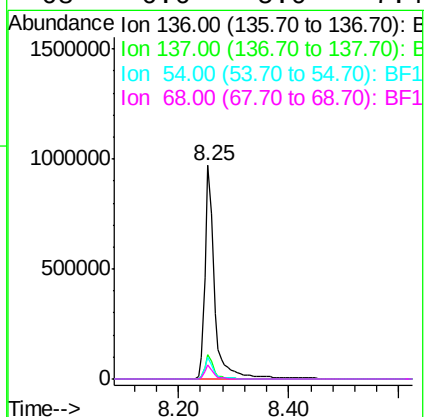
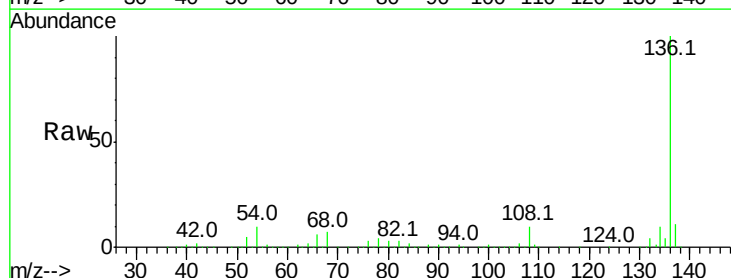


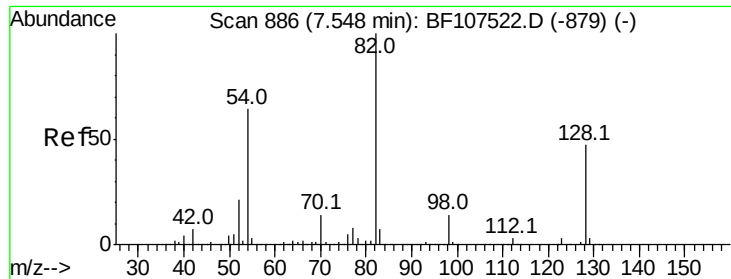

#23
Nitrobenzene-d5
Concen: 85.285 ng
RT: 7.54 min Scan# 884
Delta R.T. -0.01 min
Lab File: BF107576.D
Acq: 21 Jul 2018 15:08




Instrument :
BNA_F
ClientSampleId :
PB111309BL


Tot Ion: 82 Resp: 1455503
Ion Ratio Lower Upper
82 100
128 46.8 36.1 54.1
54 62.8 41.4 62.2#

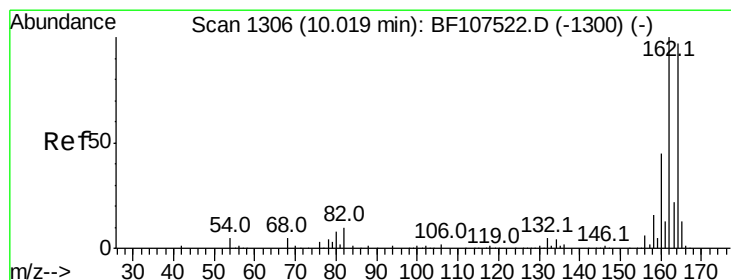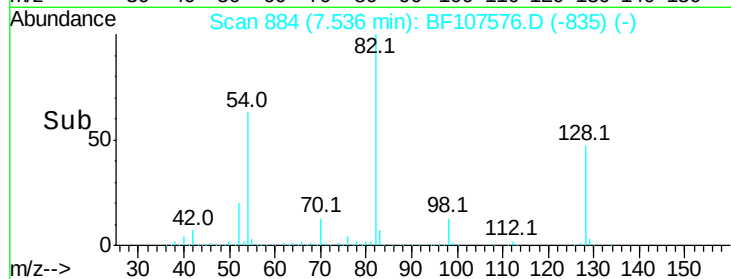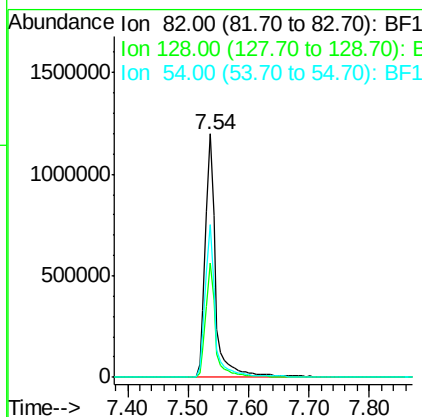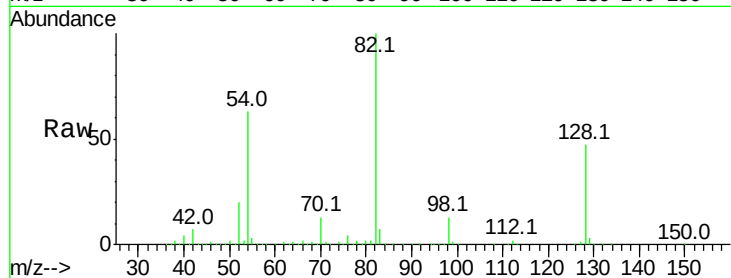

#38
Acenaphthene-d10
Concen: 20.000 ng
RT: 10.01 min Scan# 1305
Delta R.T. -0.01 min
Lab File: BF107576.D
Acq: 21 Jul 2018 15:08

Tgt Ion:164 Resp: 437112
Ion Ratio Lower Upper
164 100
162 104.4 86.1 129.1
160 47.1 38.3 57.5

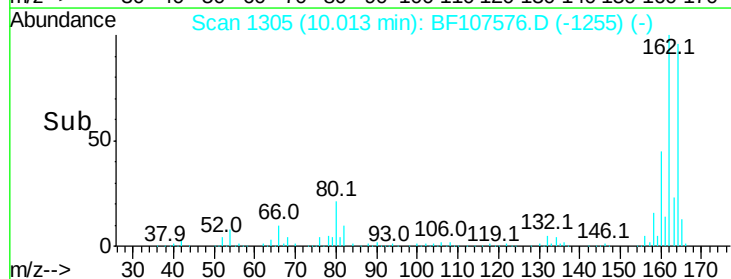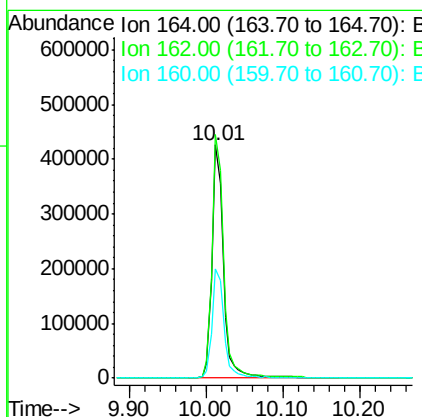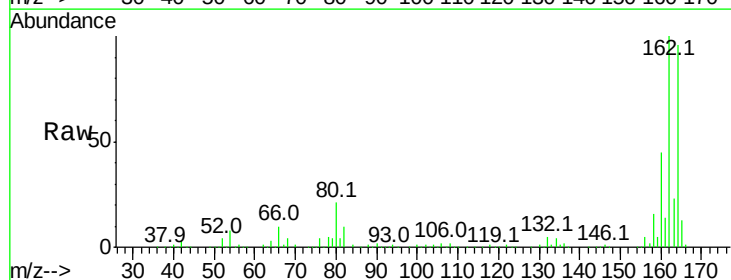


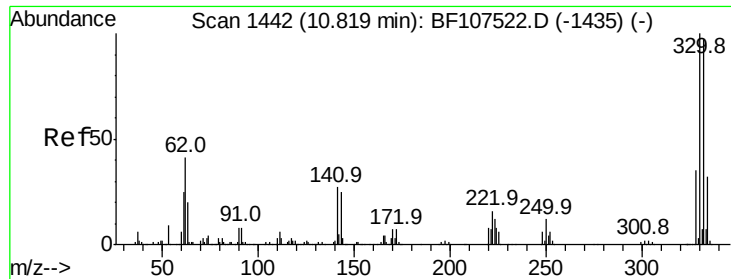




#41
 2,4,6-Tribromophenol
 Concen: 69.156 ng
 RT: 10.81 min Scan# 1440
 Delta R.T. -0.01 min
 Lab File: BF107576.D
 Acq: 21 Jul 2018 15:08

Instrument :
 BNA_F
 ClientSampleId :
 PB111309BL

Tot Ion:330 Resp: 343748
 Ion Ratio Lower Upper
 330 100
 332 95.4 77.0 115.6
 141 29.8 29.9 44.9#

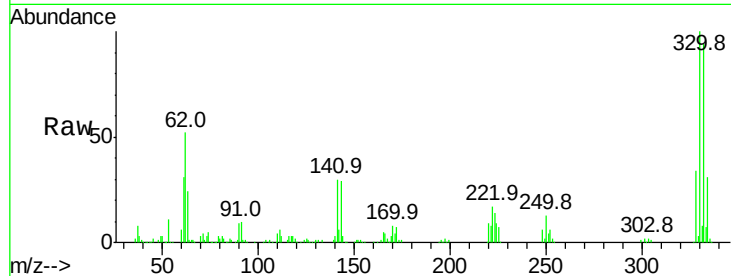


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

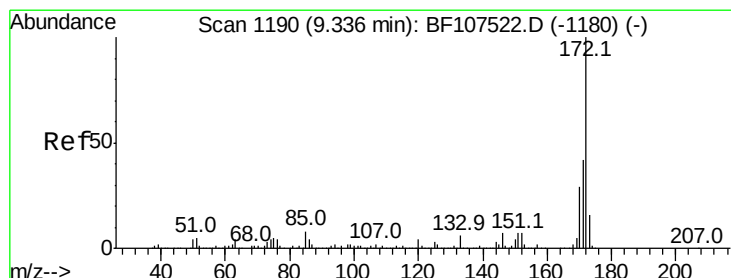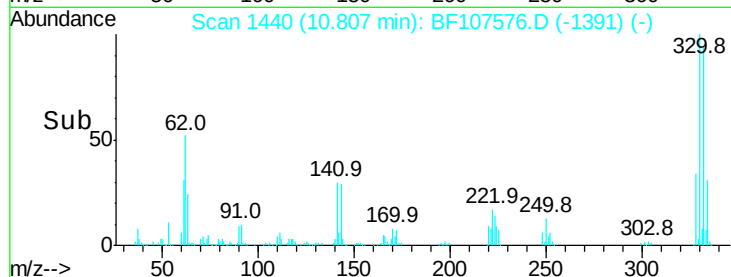
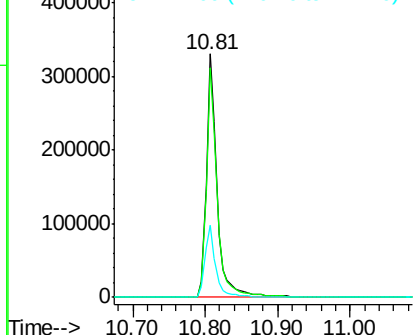



#44
 2-Fluorobiphenyl
 Concen: 101.817 ng
 RT: 9.33 min Scan# 1189
 Delta R.T. -0.01 min
 Lab File: BF107576.D
 Acq: 21 Jul 2018 15:08

Tgt Ion:172 Resp: 2463535
 Ion Ratio Lower Upper
 172 100
 171 39.5 29.7 44.5
 170 26.5 19.6 29.4

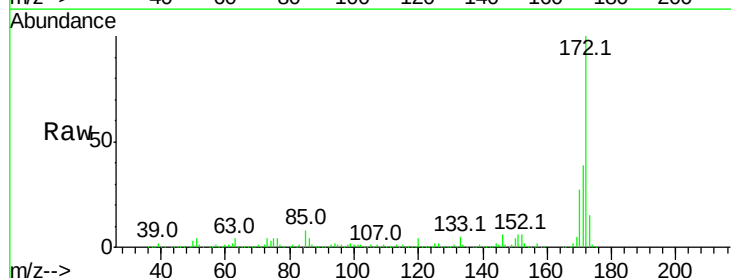

Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

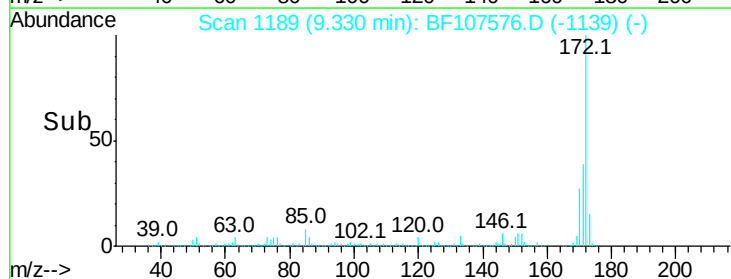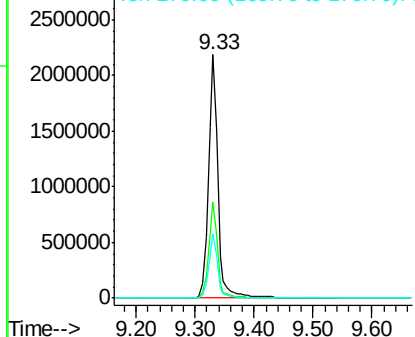

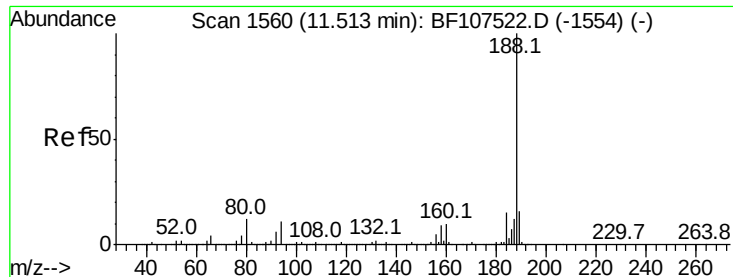

#63

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.51 min Scan# 1559

Delta R.T. -0.01 min

Lab File: BF107576.D

Acq: 21 Jul 2018 15:08

Instrument :

BNA_F

ClientSampleId :

PB111309BL


Tot Ion:188 Resp: 734989

Ion Ratio Lower Upper

188 100

94 10.9 8.5 12.7




80 11.4 9.2 13.8

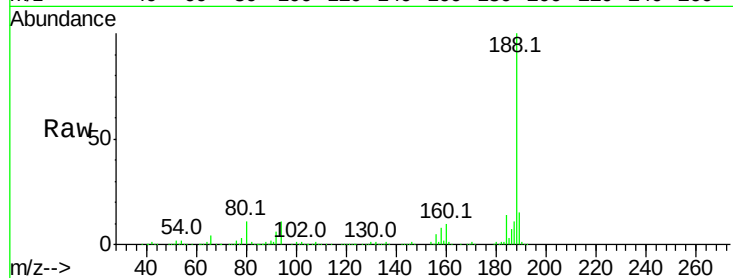

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BF1

Ion 80.00 (79.70 to 80.70): BF1

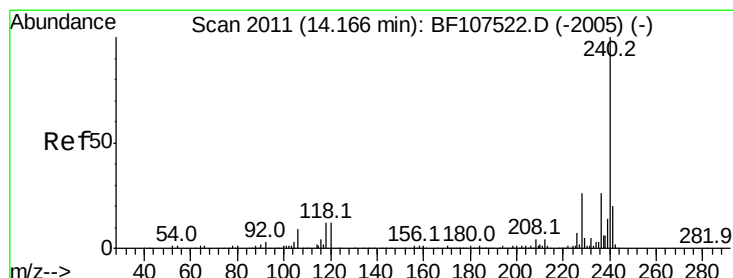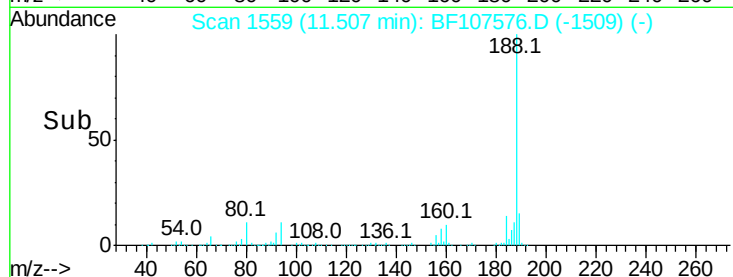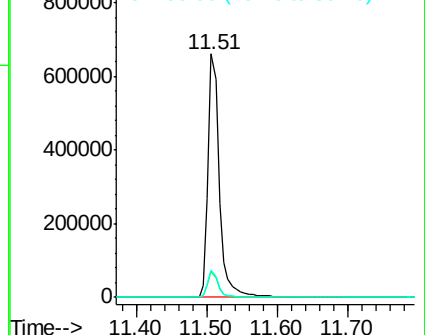

#75

Chrysene-d12

Concen: 20.000 ng

RT: 14.16 min Scan# 2010

Delta R.T. -0.01 min

Lab File: BF107576.D

Acq: 21 Jul 2018 15:08


Tgt Ion:240 Resp: 679519

Ion Ratio Lower Upper

240 100

120 12.1 9.5 14.3



236 25.2 20.7 31.1

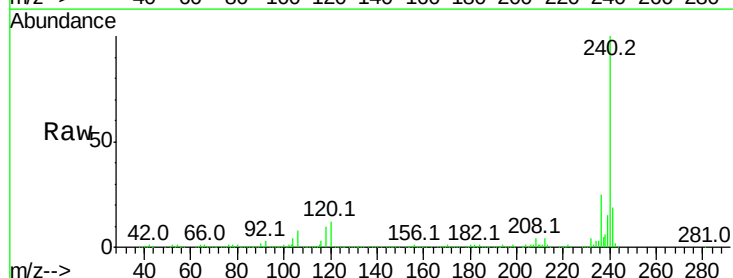


Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

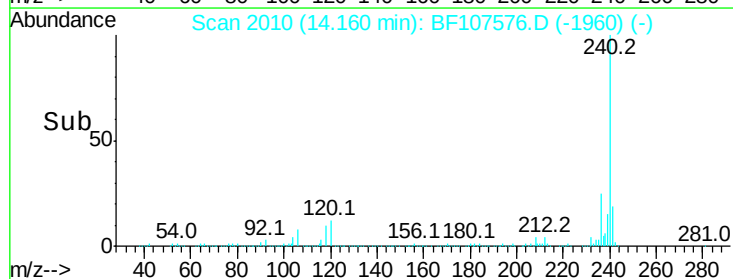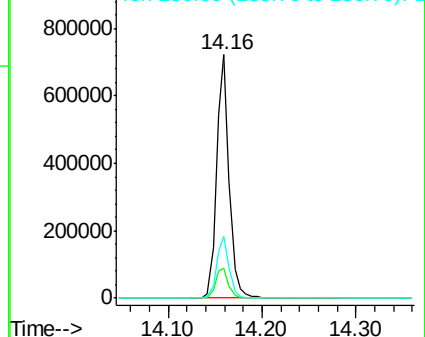

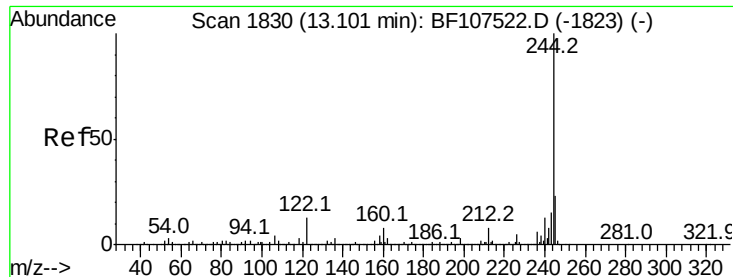

#78

Terphenyl-d14

Concen: 69.731 ng

RT: 13.09 min Scan# 1829

Delta R.T. -0.01 min

Lab File: BF107576.D

Acq: 21 Jul 2018 15:08

Instrument :


BNA_F

ClientSampleId :

PB111309BL

Tot Ion:244 Resp: 1850861




Ion	Ratio	Lower	Upper
244	100		
212	7.2	5.4	8.0
122	12.5	11.0	16.4

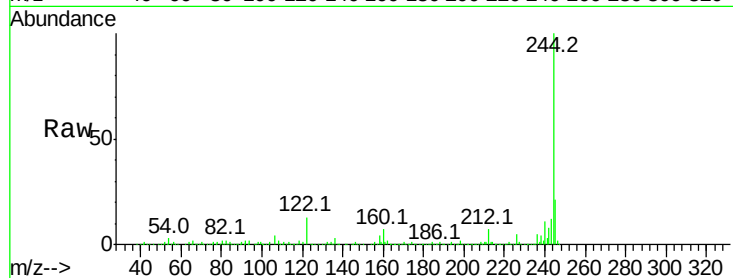

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

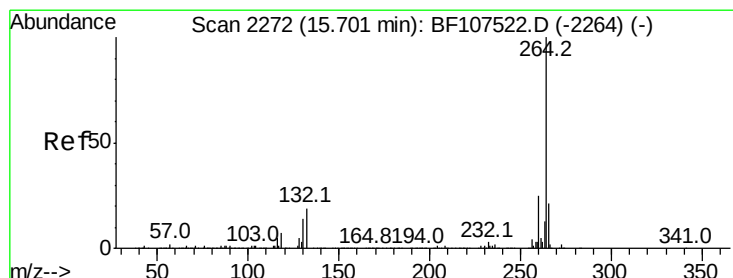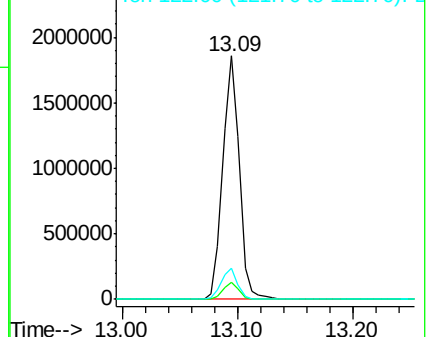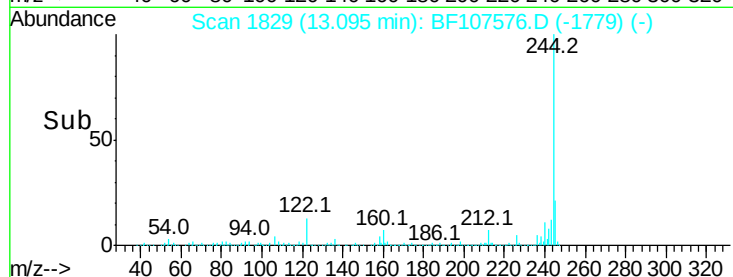

#86

Perylene-d12

Concen: 20.000 ng

RT: 15.69 min Scan# 2271


Delta R.T. -0.01 min

Lab File: BF107576.D

Acq: 21 Jul 2018 15:08

Tgt Ion:264 Resp: 558706

Ion	Ratio	Lower	Upper
264	100		
260	24.7	19.2	28.8
265	21.4	17.5	26.3

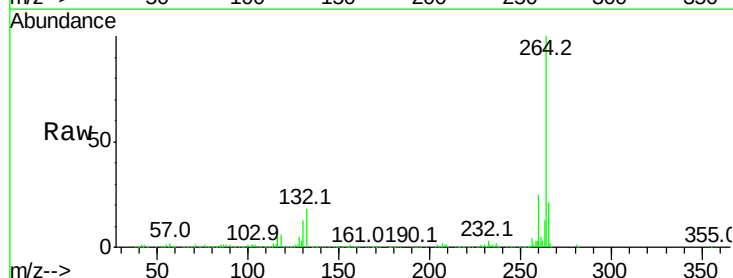

Abundance Ion 264.00 (263.70 to 264.70): E

Ion 260.00 (259.70 to 260.70): E

Ion 265.00 (264.70 to 265.70): E

