

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072018\
 Data File : BF107556.D
 Acq On : 21 Jul 2018 6:17
 Operator : JU/SJ
 Sample : J3909-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSN-001A-071918

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.201	483	487	494	rBV	269683	299967	5.85%	0.259%
2	5.572	546	550	552	rBV	325595	326732	6.37%	0.282%
3	5.601	552	555	565	rVB	1084678	1405200	27.39%	1.214%
4	5.831	590	594	607	rVB	179524	217568	4.24%	0.188%
5	6.601	721	725	735	rBV	603776	1176541	22.94%	1.016%
6	6.743	746	749	756	rBV	2474196	2688285	52.41%	2.322%
7	6.943	777	783	785	rBV2	103152	179705	3.50%	0.155%
8	6.972	785	788	793	rVV	1634545	1653405	32.23%	1.428%
9	7.013	793	795	800	rVB3	170836	259508	5.06%	0.224%
10	7.072	800	805	808	rBV2	160179	161925	3.16%	0.140%
11	7.131	808	815	823	rBV	3392689	3761548	73.33%	3.250%
12	7.237	827	833	835	rBV2	352603	409857	7.99%	0.354%
13	7.260	835	837	840	rVB2	352537	286279	5.58%	0.247%
14	7.295	840	843	847	rBV2	437093	428334	8.35%	0.370%
15	7.343	847	851	853	rBV	451553	438264	8.54%	0.379%
16	7.366	853	855	857	rVB	271855	175859	3.43%	0.152%
17	7.390	857	859	864	rVB3	149209	227282	4.43%	0.196%
18	7.442	864	868	872	rBV3	150587	174799	3.41%	0.151%
19	7.501	872	878	881	rBV	518035	711255	13.87%	0.614%
20	7.537	881	884	891	rBV2	2640957	3288909	64.12%	2.841%
21	7.595	891	894	895	rBV	320900	301025	5.87%	0.260%
22	7.613	895	897	899	rVB	392967	325472	6.35%	0.281%
23	7.660	899	905	908	rVB	467746	672841	13.12%	0.581%
24	7.701	908	912	915	rBV3	282132	396586	7.73%	0.343%
25	7.737	915	918	921	rBV	583984	547273	10.67%	0.473%
26	7.778	921	925	932	rVB3	966485	1147309	22.37%	0.991%
27	7.837	932	935	937	rBV2	322672	376977	7.35%	0.326%
28	7.866	937	940	942	rBV	516245	383343	7.47%	0.331%
29	7.890	942	944	946	rBV2	587018	508135	9.91%	0.439%
30	7.919	946	949	952	rVB2	643418	706100	13.77%	0.610%
31	7.954	952	955	958	rVB2	887140	815363	15.90%	0.704%
32	7.990	958	961	966	rBV	1531490	1426468	27.81%	1.232%
33	8.037	966	969	972	rBV2	1013196	1038178	20.24%	0.897%
34	8.119	980	983	986	rVB2	449034	427750	8.34%	0.370%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072018\
 Data File : BF107556.D
 Acq On : 21 Jul 2018 6:17
 Operator : JU/SJ
 Sample : J3909-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSN-001A-071918

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0

Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

35	8.154	986	989	992	rBV2	539446	740671	14.44%	0.640%
36	8.201	995	997	998	rBV	333731	277914	5.42%	0.240%
37	8.225	998	1001	1004	rBV	2630611	2210202	43.09%	1.909%
38	8.260	1004	1007	1011	rBV	1499433	1509318	29.42%	1.304%
39	8.301	1011	1014	1017	rVB	3922382	3500627	68.24%	3.024%
40	8.337	1017	1020	1022	rBV2	811128	1069852	20.86%	0.924%
41	8.395	1027	1030	1033	rVB3	521541	529364	10.32%	0.457%
42	8.437	1033	1037	1038	rBV3	476031	599950	11.70%	0.518%
43	8.454	1038	1040	1043	rVB2	408878	332775	6.49%	0.287%
44	8.542	1051	1055	1059	rVB2	2285000	3016694	58.81%	2.606%
45	8.584	1059	1062	1065	rBV3	1326685	1257694	24.52%	1.087%
46	8.619	1065	1068	1072	rVV	2306372	2171364	42.33%	1.876%
47	8.666	1072	1076	1079	rVV	5180726	5129559	100.00%	4.432%
48	8.689	1079	1080	1087	rVB3	830747	1164302	22.70%	1.006%
49	8.754	1089	1091	1094	rVB3	333562	303642	5.92%	0.262%
50	8.789	1094	1097	1099	rBV	656468	732123	14.27%	0.633%
51	8.837	1101	1105	1109	rVV	4003529	3927197	76.56%	3.393%
52	8.889	1109	1114	1118	rVV3	969541	2415505	47.09%	2.087%
53	8.931	1118	1121	1124	rVV	2011939	2077198	40.49%	1.795%
54	8.960	1124	1126	1130	rVV3	281592	337559	6.58%	0.292%
55	8.995	1130	1132	1135	rVB2	495341	436859	8.52%	0.377%
56	9.031	1135	1138	1144	rBV2	1185719	1500141	29.25%	1.296%
57	9.095	1147	1149	1150	rVB	311087	184297	3.59%	0.159%
58	9.119	1150	1153	1154	rBV	1271088	1239986	24.17%	1.071%
59	9.131	1154	1155	1157	rVV	1200926	1037872	20.23%	0.897%
60	9.160	1157	1160	1163	rVB3	1822658	2140630	41.73%	1.849%
61	9.201	1163	1167	1171	rBV	2005380	1949193	38.00%	1.684%
62	9.242	1171	1174	1175	rVV	1451479	1304887	25.44%	1.127%
63	9.266	1175	1178	1181	rVV	4338417	3588491	69.96%	3.100%
64	9.331	1184	1189	1193	rBV	3951591	3872659	75.50%	3.346%
65	9.401	1198	1201	1206	rVV	4063990	4936985	96.25%	4.265%
66	9.442	1206	1208	1212	rVV	1113215	1490194	29.05%	1.287%
67	9.478	1212	1214	1216	rVV	716218	666394	12.99%	0.576%
68	9.513	1218	1220	1224	rVV3	482490	514748	10.03%	0.445%
69	9.554	1224	1227	1230	rVV4	313758	480525	9.37%	0.415%
70	9.589	1230	1233	1235	rVV2	417252	459104	8.95%	0.397%
71	9.654	1238	1244	1246	rVV2	844390	1332686	25.98%	1.151%

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072018\
 Data File : BF107556.D
 Acq On : 21 Jul 2018 6:17
 Operator : JU/SJ
 Sample : J3909-01
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DSN-001A-071918

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 3 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

72	9.678	1246	1248	1251	rVV2	786562	750504	14.63%	0.648%
73	9.719	1251	1255	1258	rVV3	4099929	4819369	93.95%	4.164%
74	9.778	1262	1265	1268	rVB	920882	713275	13.91%	0.616%
75	9.825	1268	1273	1278	rVB3	411759	615042	11.99%	0.531%
76	9.878	1278	1282	1284	rBV	294147	308201	6.01%	0.266%
77	9.931	1287	1291	1295	rVB	1696824	1709603	33.33%	1.477%
78	9.972	1295	1298	1300	rBV2	358500	378107	7.37%	0.327%
79	10.019	1303	1306	1309	rVB	1380901	1083970	21.13%	0.936%
80	10.160	1326	1330	1333	rVV2	337759	505877	9.86%	0.437%
81	10.189	1333	1335	1337	rVV	448296	358640	6.99%	0.310%
82	10.219	1337	1340	1342	rVV	291295	254997	4.97%	0.220%
83	10.248	1342	1345	1350	rVV2	631420	771005	15.03%	0.666%
84	10.289	1350	1352	1356	rVB	245528	202084	3.94%	0.175%
85	10.431	1372	1376	1379	rVV	563053	504690	9.84%	0.436%
86	10.648	1408	1413	1416	rBV	435045	447265	8.72%	0.386%
87	10.807	1437	1440	1449	rBV	1816334	1875052	36.55%	1.620%
88	10.913	1454	1458	1462	rBV	283900	362776	7.07%	0.313%
89	11.513	1556	1560	1568	rBV	1579694	1646905	32.11%	1.423%
90	12.019	1643	1646	1651	rBV	448428	449318	8.76%	0.388%
91	13.095	1825	1829	1837	rBV	5281180	4915222	95.82%	4.246%
92	13.213	1846	1849	1858	rBV	368583	460030	8.97%	0.397%
93	13.977	1975	1979	1986	rBV	265778	309674	6.04%	0.268%
94	14.160	2006	2010	2016	rBV	2119461	2024465	39.47%	1.749%
95	14.601	2082	2085	2091	rVB	150137	161169	3.14%	0.139%
96	14.924	2137	2140	2147	rVB	176857	174531	3.40%	0.151%
97	15.007	2150	2154	2159	rVB	149267	162153	3.16%	0.140%
98	15.277	2197	2200	2204	rBV	174926	209390	4.08%	0.181%
99	15.689	2265	2270	2278	rBV	1098570	1577461	30.75%	1.363%
100	16.148	2344	2348	2354	rBV	141758	216526	4.22%	0.187%


Sum of corrected areas: 115750504

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072018\
Data File : BF107556.D
Acq On : 21 Jul 2018 6:17
Operator : JU/SJ
Sample : J3909-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN-001A-071918

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

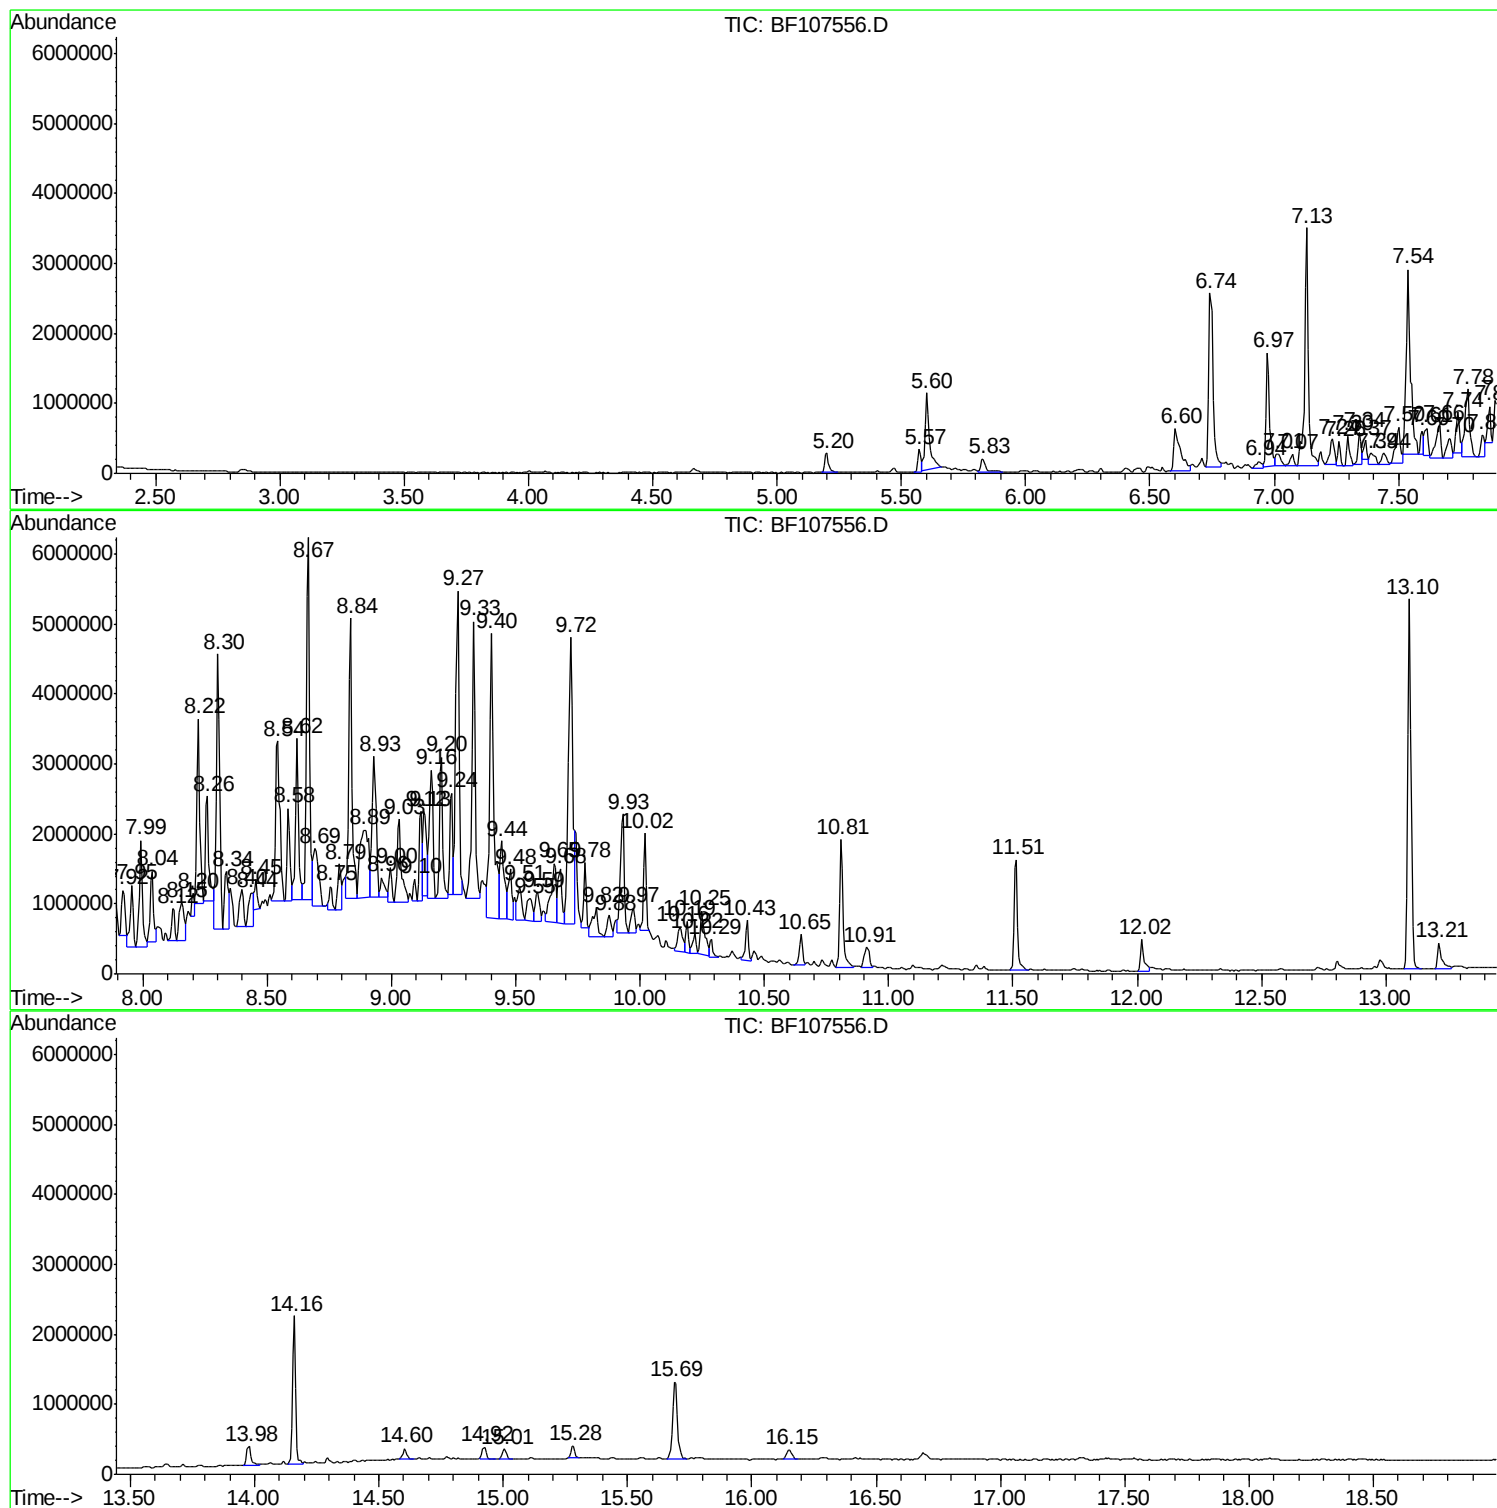

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072018\
Data File : BF107556.D
Acq On : 21 Jul 2018 6:17
Operator : JU/SJ
Sample : J3909-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN-001A-071918

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072018\
Data File : BF107556.D
Acq On : 21 Jul 2018 6:17
Operator : JU/SJ
Sample : J3909-01
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DSN-001A-071918

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---
					# RT Resp Conc