


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072018\
 Data File : BF107527.D
 Acq On : 20 Jul 2018 16:55
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 16:29:27 2018

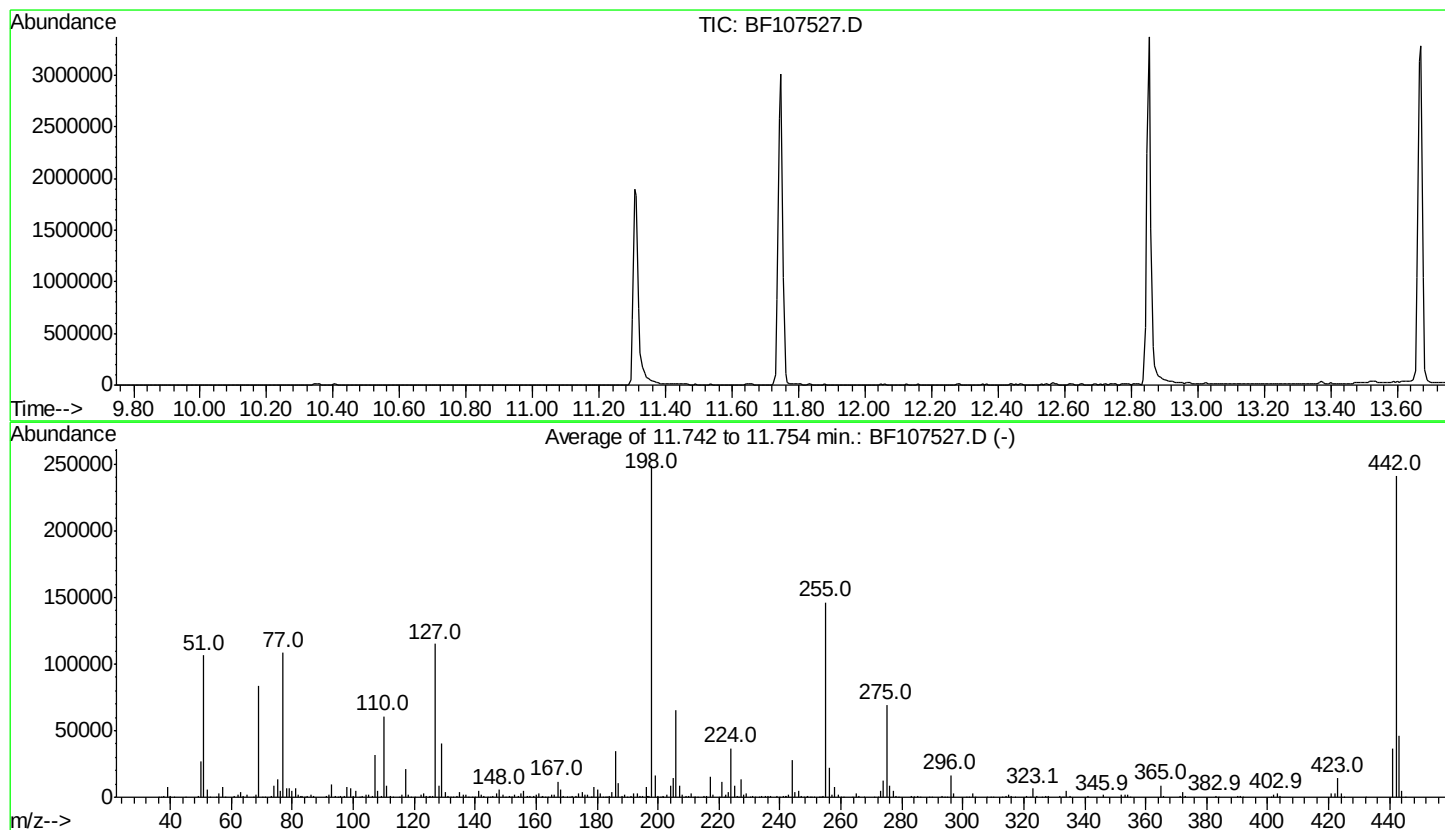

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	106261	PASS
68	69	0.00	2	1.8	1503	PASS
69	198	0.00	100	33.6	83736	PASS
70	69	0.00	2	0.6	487	PASS
127	198	10	80	46.3	115165	PASS
197	198	0.00	2	0.5	1167	PASS
198	198	100	100	100.0	248960	PASS
199	198	5	9	6.6	16494	PASS
275	198	10	60	27.9	69368	PASS
365	198	1	100	3.6	8911	PASS
441	198	0.01	100	14.8	36938	PASS
442	198	50	100	96.9	241258	PASS
443	442	15	24	19.3	46485	PASS