
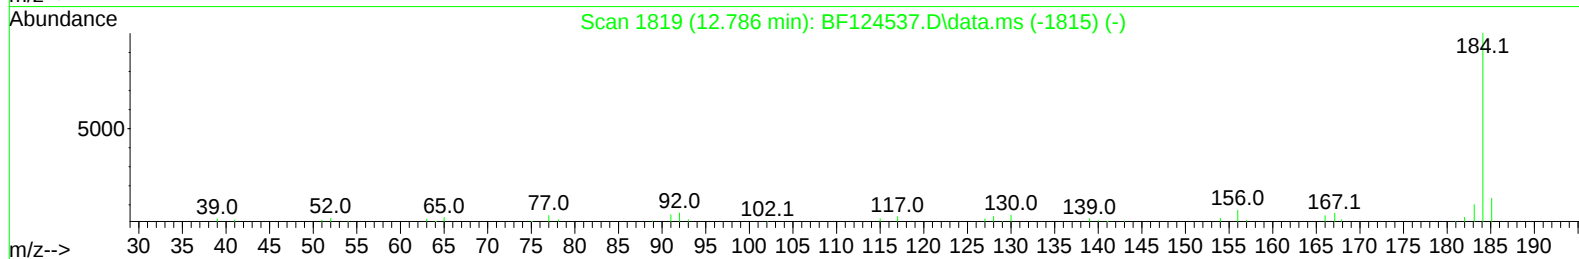
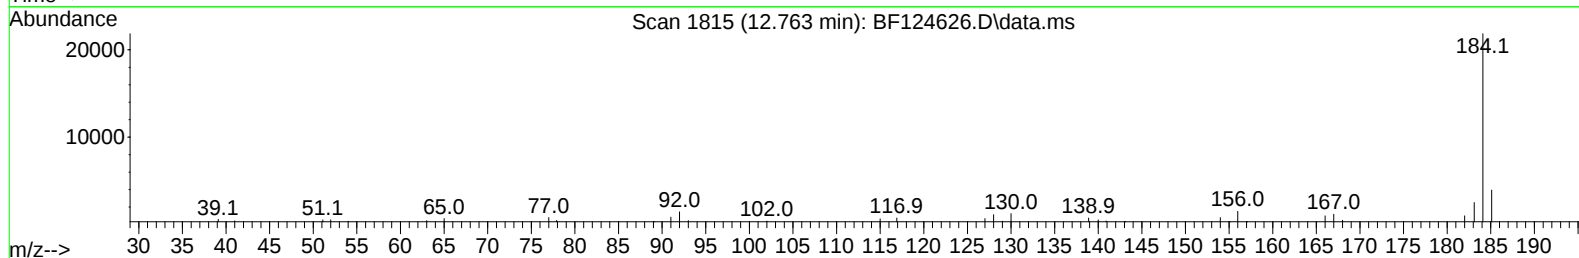


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
 Data File : BF124626.D
 Acq On : 20 Jul 2021 11:09
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 11:46:38 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Jul 19 11:33:09 2021
 Response via : Initial Calibration

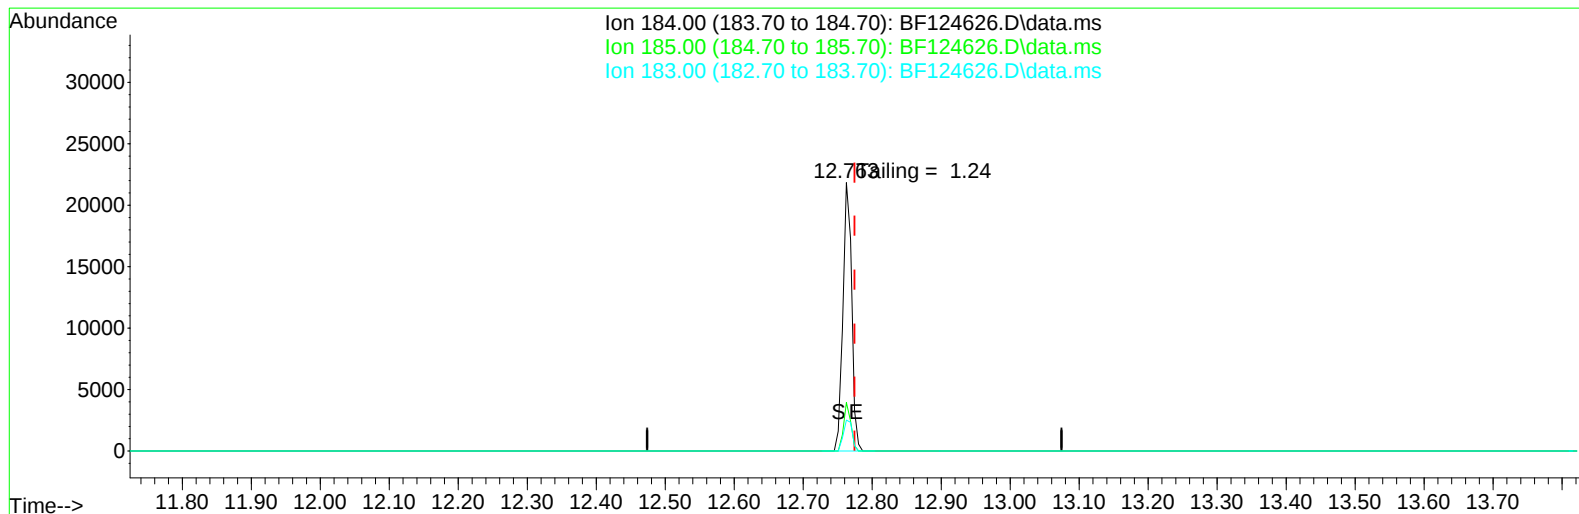

TIC: BF124626.D\data.ms

(77) Benzidine




12.763min (-0.012) 0.00 ng

response 19214

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	18.08#
183.00	10.10	11.52
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124626.D
Acq On : 20 Jul 2021 11:09
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 11:46:38 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 19 11:33:09 2021
Response via : Initial Calibration

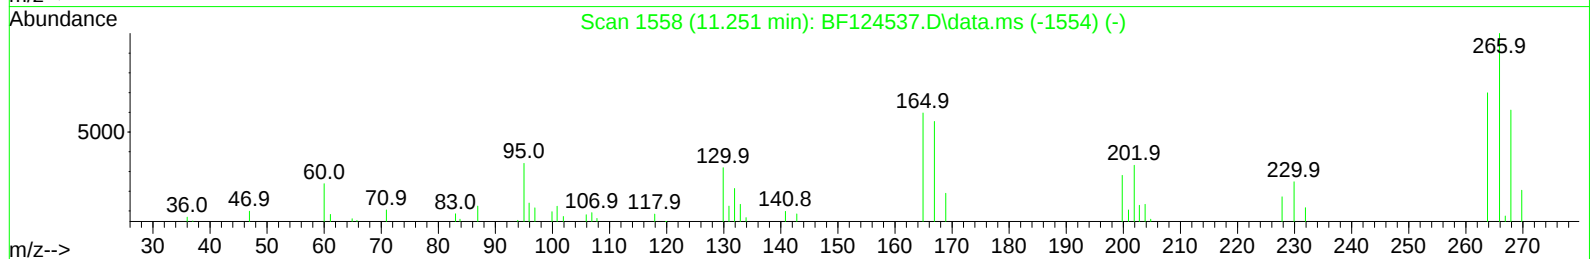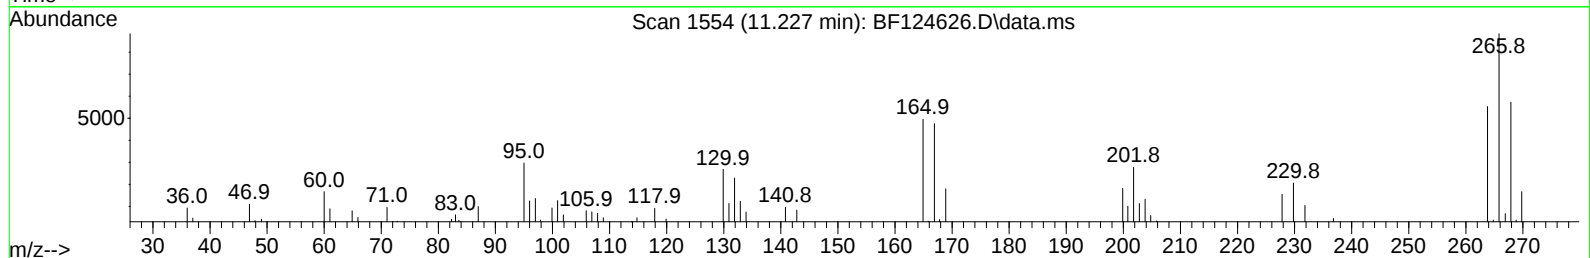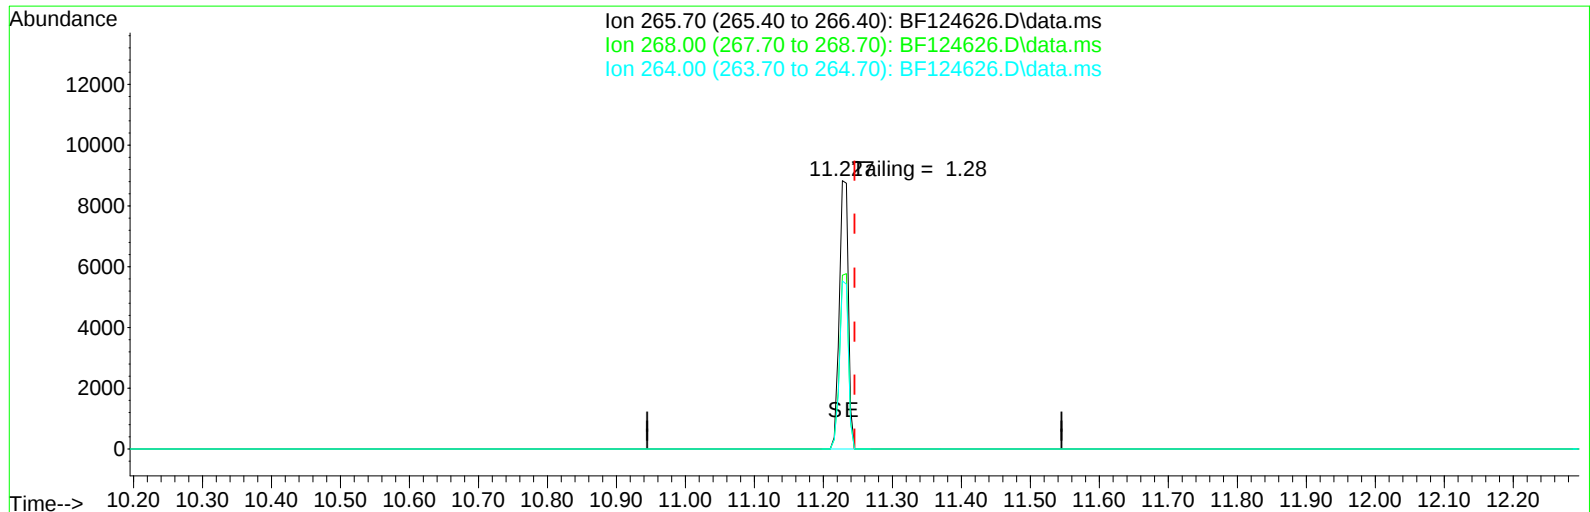

TIC: BF124626.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.018) 0.00 ng

response 8004

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	64.78
264.00	69.90	62.63
0.00	0.00	0.00