

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
 Data File : BF124628.D
 Acq On : 20 Jul 2021 13:25
 Operator : JU/CG
 Sample : PB137770BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137770BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124628.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.187	524	527	532	rBB2	4026	5209	1.39%	0.251%
2	5.539	581	587	590	rBB	235485	290987	77.54%	14.010%
3	6.528	748	755	758	rBB	214267	297006	79.14%	14.299%
4	6.904	816	819	822	rBB	57475	47256	12.59%	2.275%
5	7.469	909	915	917	rBB	165589	188364	50.19%	9.069%
6	8.186	1032	1037	1040	rBB	67598	65341	17.41%	3.146%
7	9.269	1214	1221	1224	rBB	366332	375294	100.00%	18.068%
8	9.945	1331	1336	1339	rBB	87312	73939	19.70%	3.560%
9	10.733	1465	1470	1473	rBV	204914	222208	59.21%	10.698%
10	11.433	1585	1589	1592	rVB	84244	72800	19.40%	3.505%
11	13.021	1854	1859	1862	rBV	332342	358733	95.59%	17.271%
12	14.068	2033	2037	2040	rBB	58154	46708	12.45%	2.249%
13	15.556	2285	2290	2294	rBB	28904	33221	8.85%	1.599%




Sum of corrected areas: 2077066

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124628.D
Acq On : 20 Jul 2021 13:25
Operator : JU/CG
Sample : PB137770BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137770BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

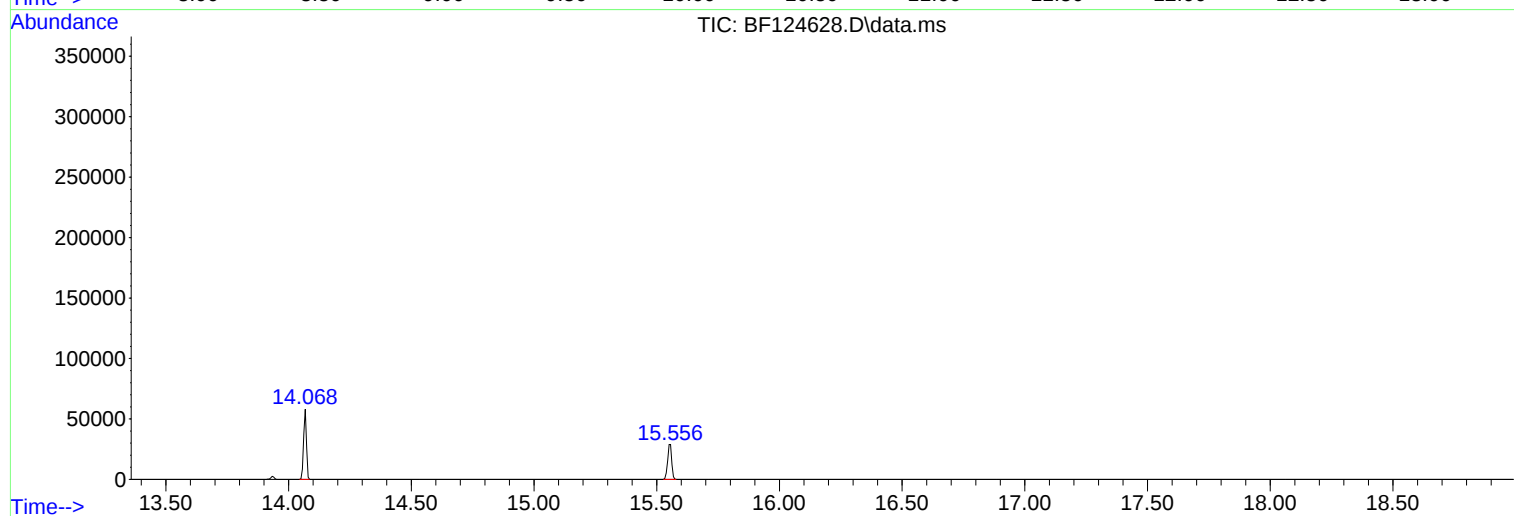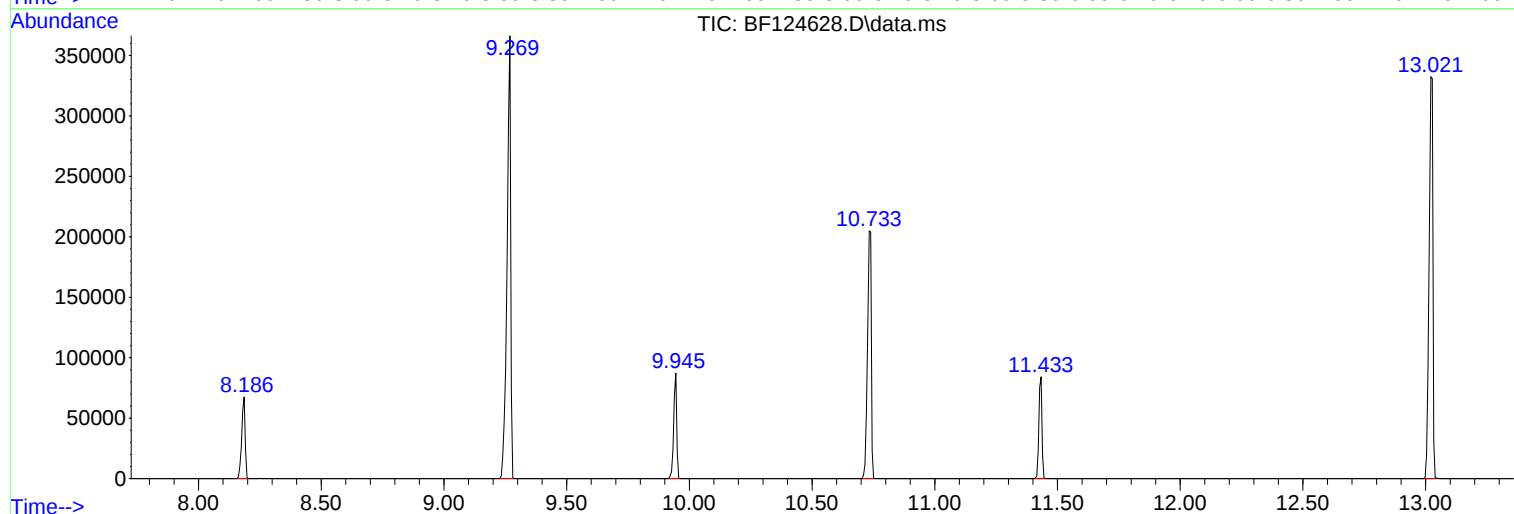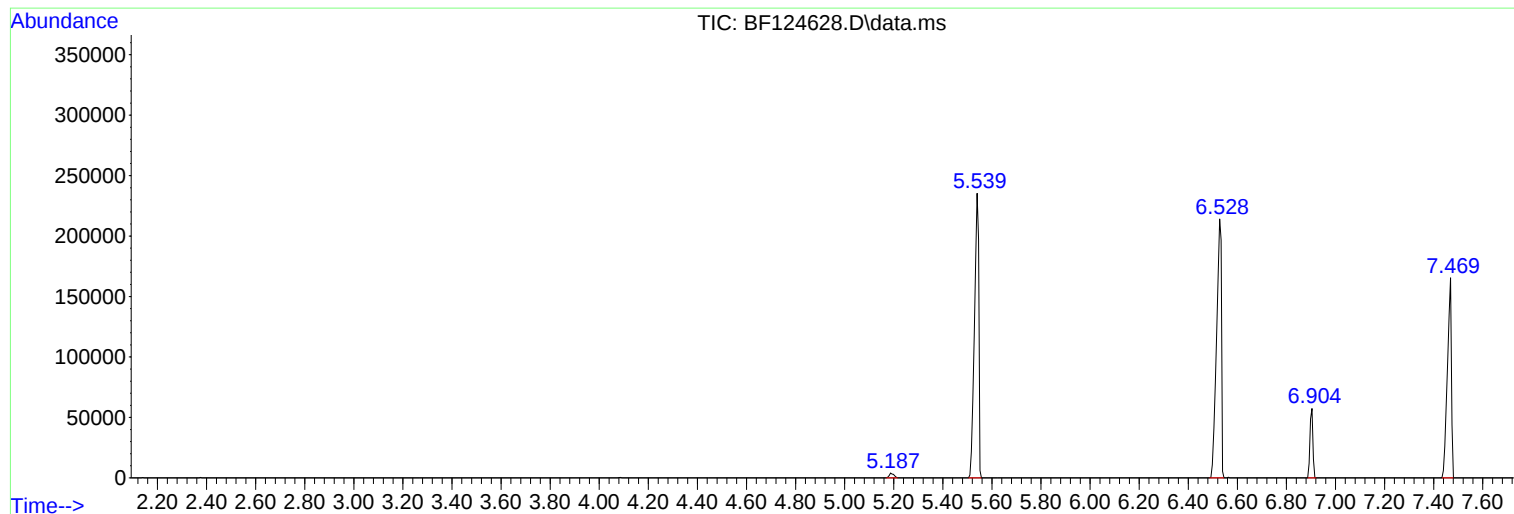

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124628.D
Acq On : 20 Jul 2021 13:25
Operator : JU/CG
Sample : PB137770BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137770BL








Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown5.187 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.187	2.20 ng	5209	1,4-Dichlorobenzene-d4	6.904

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diacetamide	101	C4H7NO2	000625-77-4	3
2			2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	3
3			Isopropyl isothiocyanate	101	C4H7NS	002253-73-8	3
4			.alpha.-Amino-.gamma.-butyrolactone	101	C4H7NO2	001192-20-7	3
5			N-(n-Propyl)acetamide	101	C5H11NO	005331-48-6	3

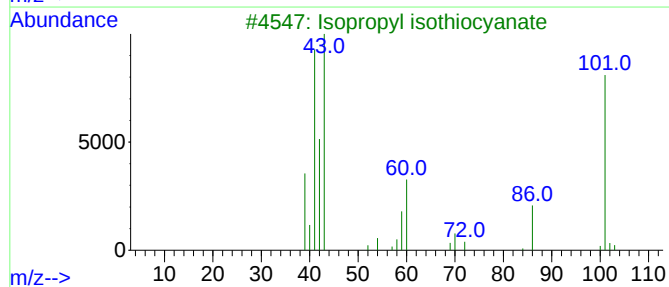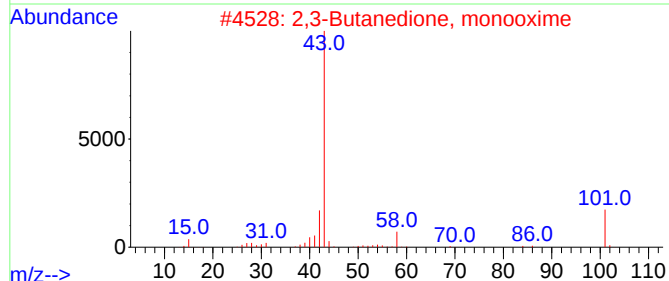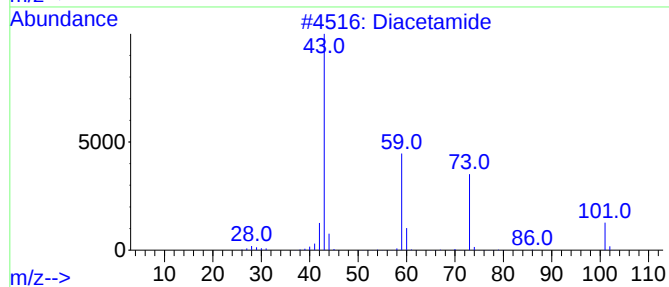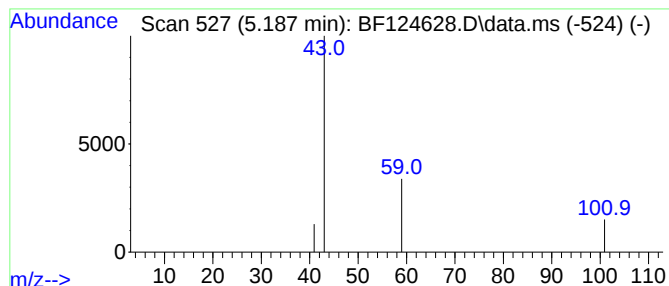

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124628.D
Acq On : 20 Jul 2021 13:25
Operator : JU/CG
Sample : PB137770BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137770BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
unknown5.187	5.187	2.2	ng	5209	1	6.904	47256	20.0