

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
 Data File : BF124638.D
 Acq On : 20 Jul 2021 20:53
 Operator : JU/CG
 Sample : PB137705BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB137705BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124638.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.157	519	522	526	rBB	2610	3269	1.26%	0.224%
2	5.528	580	585	588	rBB	192834	194758	75.02%	13.361%
3	6.522	748	754	757	rBB	168850	200198	77.12%	13.734%
4	6.898	815	818	821	rBB	43479	37358	14.39%	2.563%
5	7.463	909	914	917	rBB	122421	130220	50.16%	8.933%
6	8.186	1032	1037	1040	rBB	56849	52987	20.41%	3.635%
7	9.263	1215	1220	1223	rBB	284621	259602	100.00%	17.809%
8	9.939	1331	1335	1339	rBB	68101	62740	24.17%	4.304%
9	10.733	1465	1470	1473	rBB	174206	150634	58.02%	10.334%
10	11.433	1585	1589	1592	rBB	68618	62158	23.94%	4.264%
11	13.021	1854	1859	1862	rBV	277816	241253	92.93%	16.550%
12	14.068	2034	2037	2040	rVB	44617	35348	13.62%	2.425%
13	15.551	2285	2289	2293	rBV	22419	27162	10.46%	1.863%




Sum of corrected areas: 1457687

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124638.D
Acq On : 20 Jul 2021 20:53
Operator : JU/CG
Sample : PB137705BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137705BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

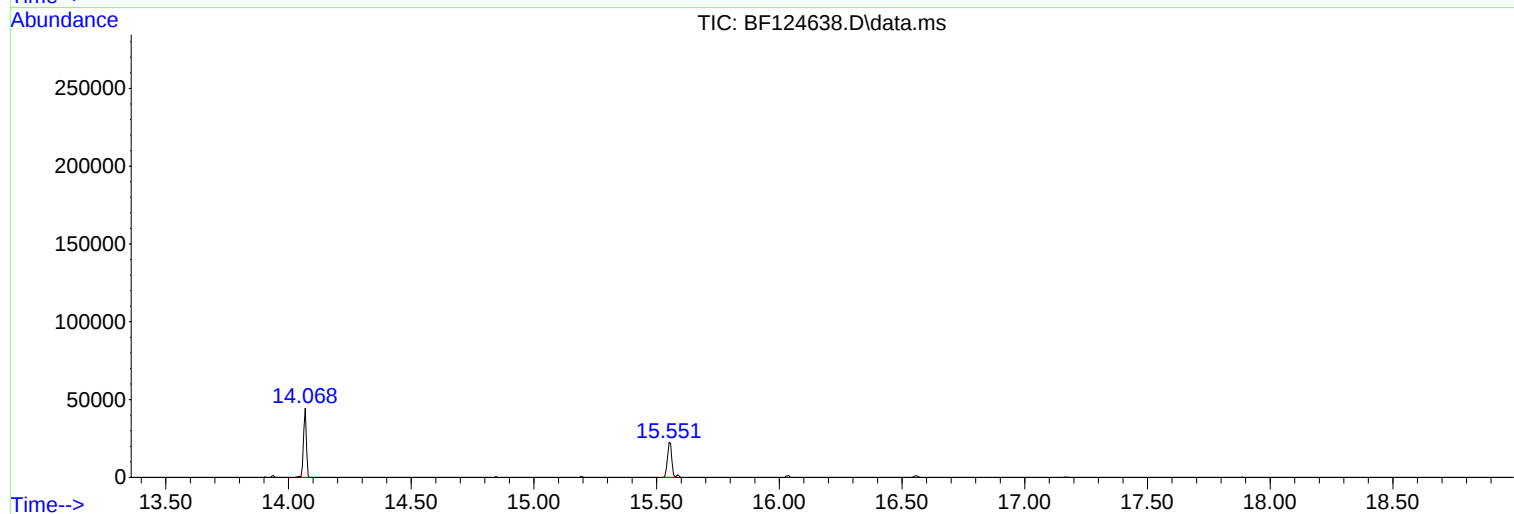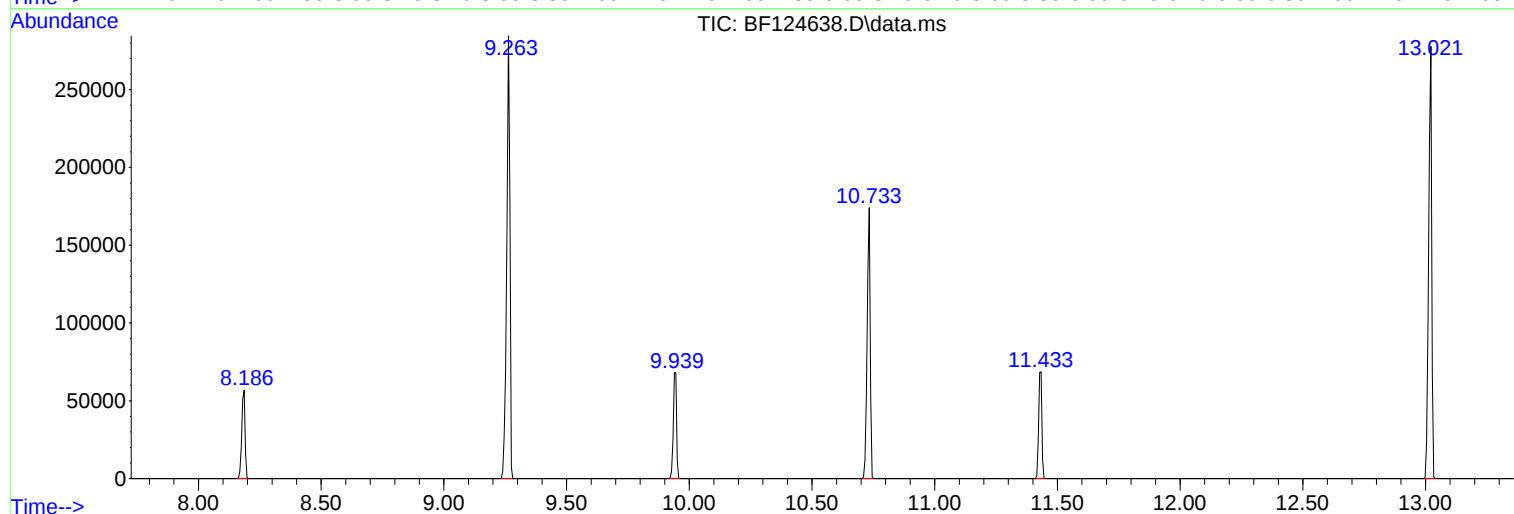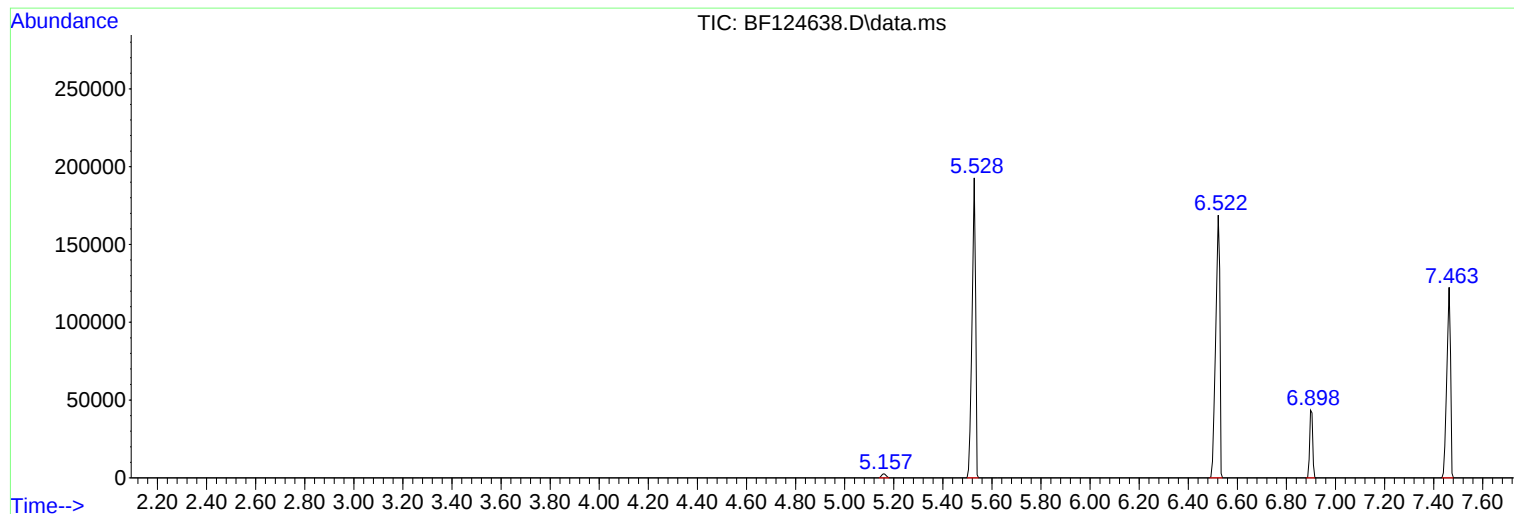

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124638.D
Acq On : 20 Jul 2021 20:53
Operator : JU/CG
Sample : PB137705BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137705BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124638.D
Acq On : 20 Jul 2021 20:53
Operator : JU/CG
Sample : PB137705BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB137705BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------