

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
 Data File : BF124639.D
 Acq On : 20 Jul 2021 21:32
 Operator : JU/CG
 Sample : M3061-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB-2021-WS-000-08

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF124639.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.522	72	74	76	rVB	531016	371989	100.00%	17.838%
2	2.993	150	154	159	rBB	12578	16397	4.41%	0.786%
3	4.734	447	450	453	rBB	19932	18163	4.88%	0.871%
4	5.151	516	521	527	rBB2	26194	44635	12.00%	2.140%
5	5.534	581	586	589	rBB	177122	188388	50.64%	9.034%
6	6.528	749	755	758	rBB	164144	174518	46.91%	8.369%
7	6.904	816	819	822	rBB	52196	39405	10.59%	1.890%
8	7.463	909	914	917	rBB	125826	139403	37.48%	6.685%
9	8.187	1033	1037	1040	rBB	63664	57152	15.36%	2.741%
10	9.263	1215	1220	1223	rBB	300701	278219	74.79%	13.341%
11	9.939	1332	1335	1339	rBB	76812	68914	18.53%	3.305%
12	10.733	1465	1470	1473	rBB	198280	181691	48.84%	8.713%
13	11.428	1585	1588	1592	rVB	81926	70697	19.01%	3.390%
14	11.951	1671	1677	1680	rBV	40575	45283	12.17%	2.171%
15	12.733	1806	1810	1814	rBB	22438	20385	5.48%	0.978%
16	13.022	1854	1859	1862	rBV	308147	296787	79.78%	14.232%
17	13.933	2011	2014	2017	rVB	5863	6821	1.83%	0.327%
18	14.069	2033	2037	2040	rVB	53814	42386	11.39%	2.033%
19	15.551	2285	2289	2292	rBV	21210	24146	6.49%	1.158%




Sum of corrected areas: 2085379

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124639.D
Acq On : 20 Jul 2021 21:32
Operator : JU/CG
Sample : M3061-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB-2021-WS-000-08

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

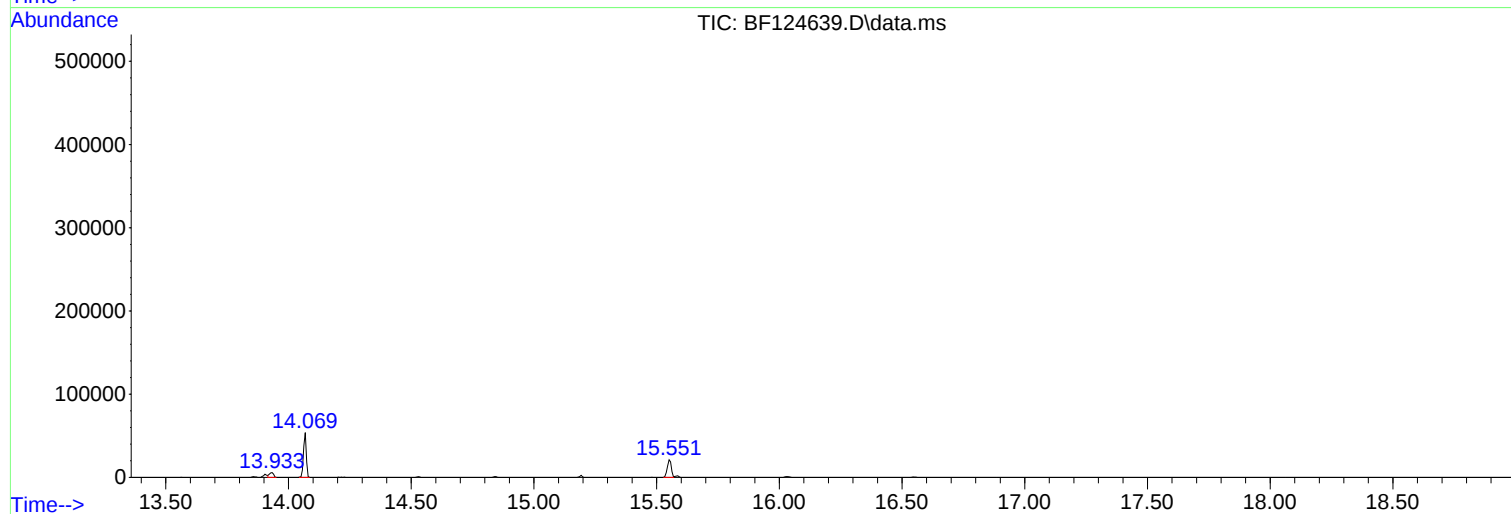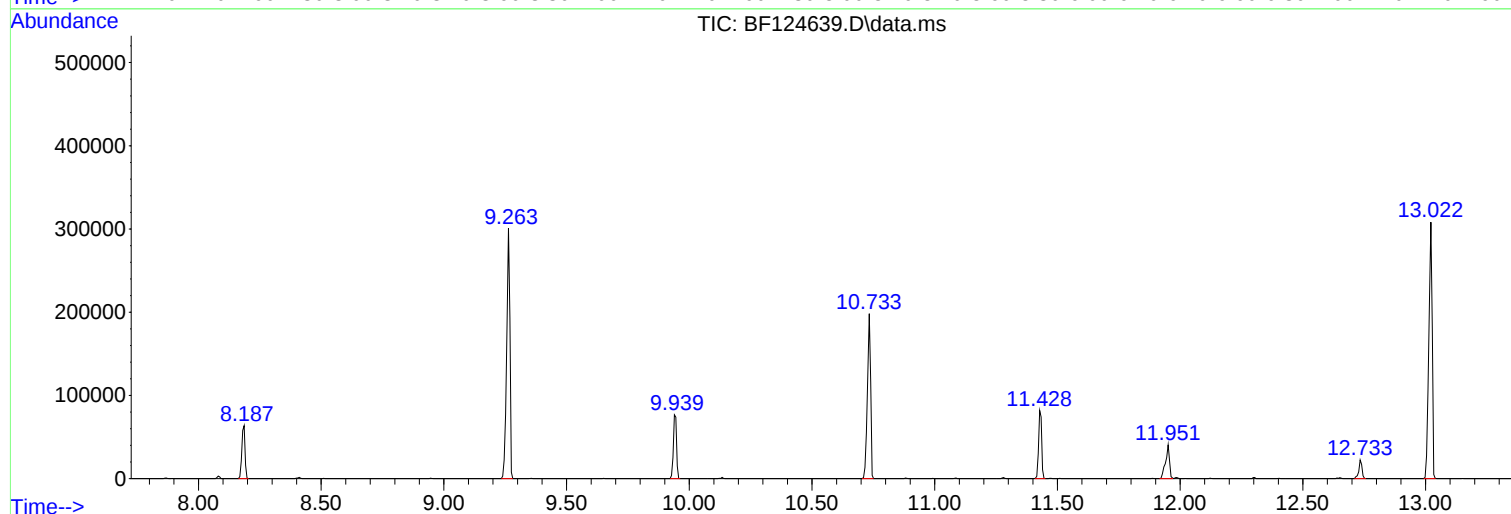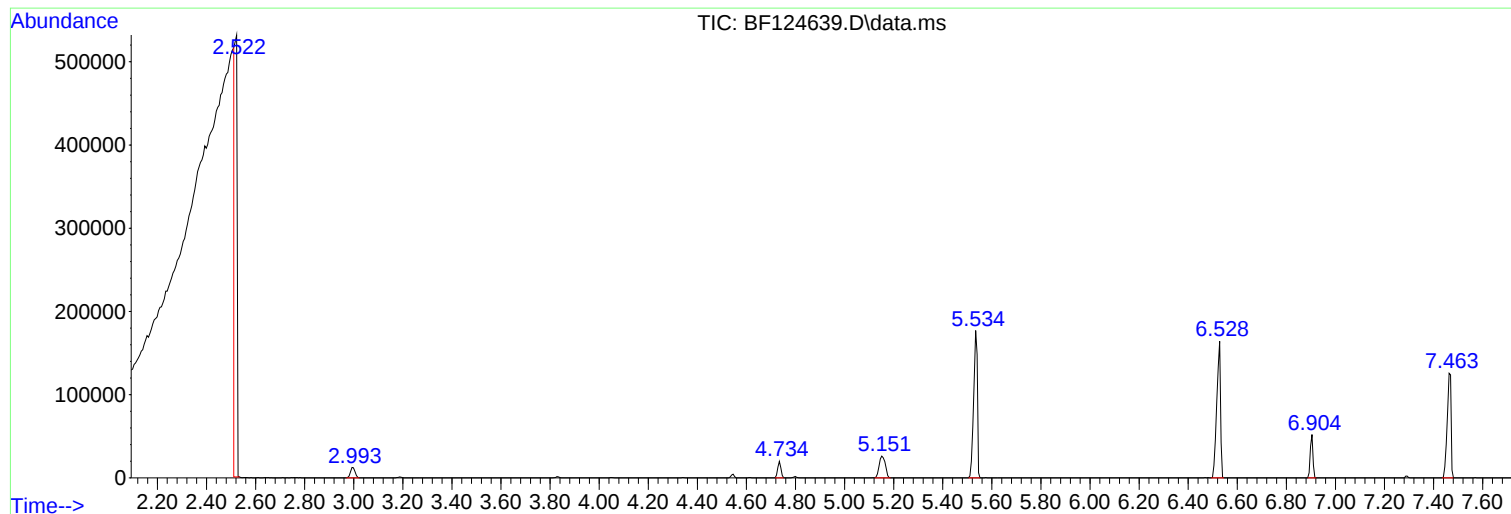

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124639.D
Acq On : 20 Jul 2021 21:32
Operator : JU/CG
Sample : M3061-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB-2021-WS-000-08

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
Data File : BF124639.D
Acq On : 20 Jul 2021 21:32
Operator : JU/CG
Sample : M3061-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB-2021-WS-000-08

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
