
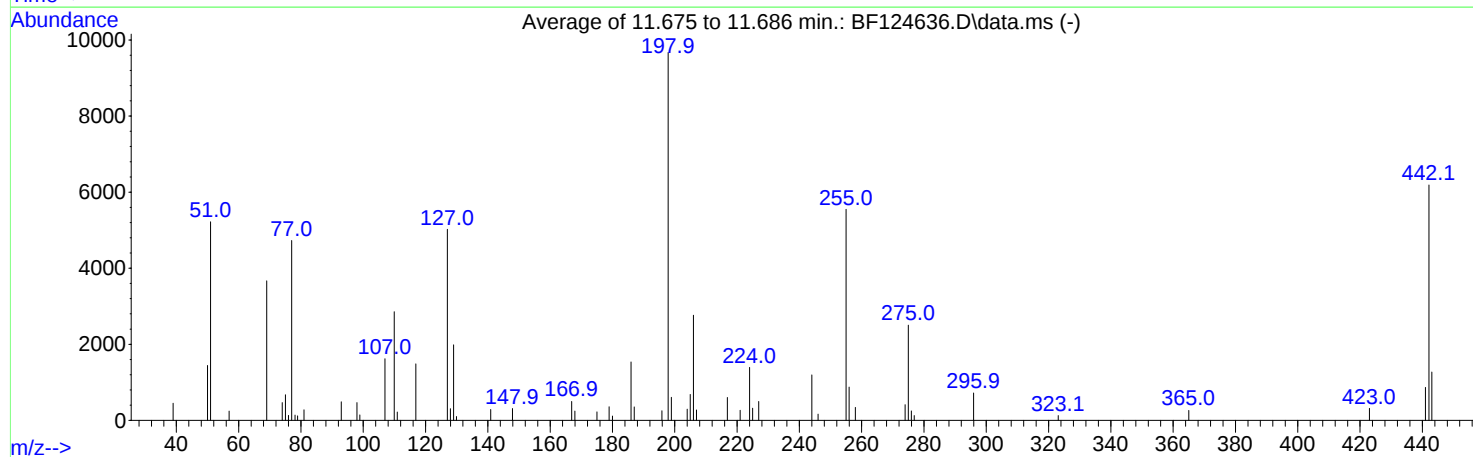


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
 Data File : BF124636.D
 Acq On : 20 Jul 2021 19:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jul 20 13:36:28 2021

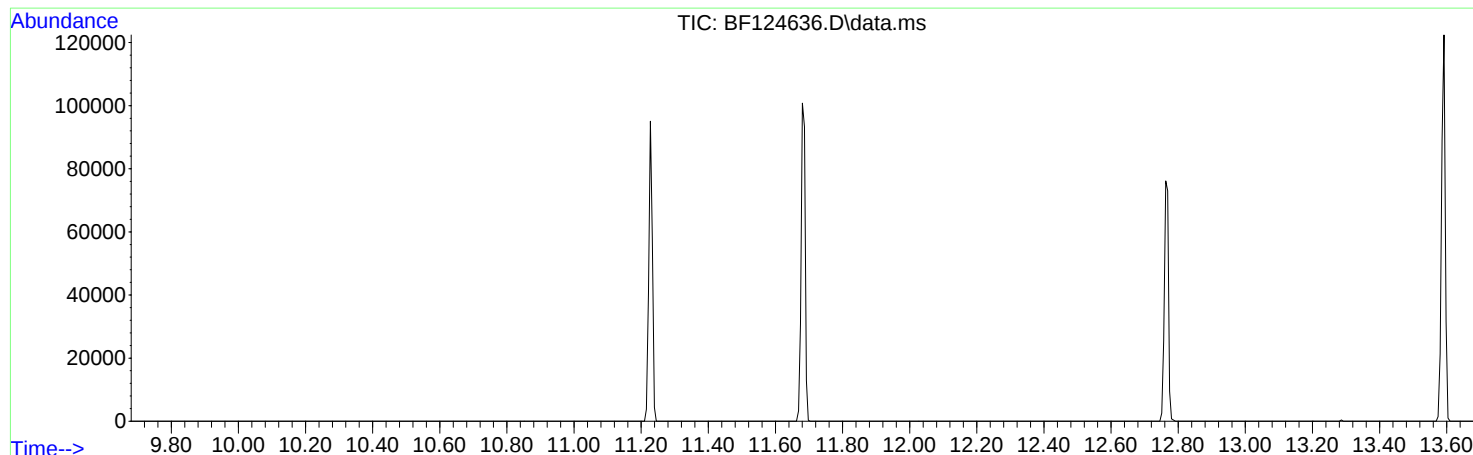




AutoFind: Scans 1630, 1631, 1632; Background Corrected with Scan 1626

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.0	5219	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	37.9	3670	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.9	5022	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	9671	PASS
199	198	5	9	6.3	605	PASS
275	198	10	60	25.9	2504	PASS
365	198	1	100	2.7	262	PASS
441	198	0.01	100	9.0	868	PASS
442	442	50	100	100.0	6189	PASS
443	442	15	24	20.5	1269	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
 Data File : BF124636.D
 Acq On : 20 Jul 2021 19:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 21 05:28:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 20 13:36:28 2021
 Response via : Initial Calibration

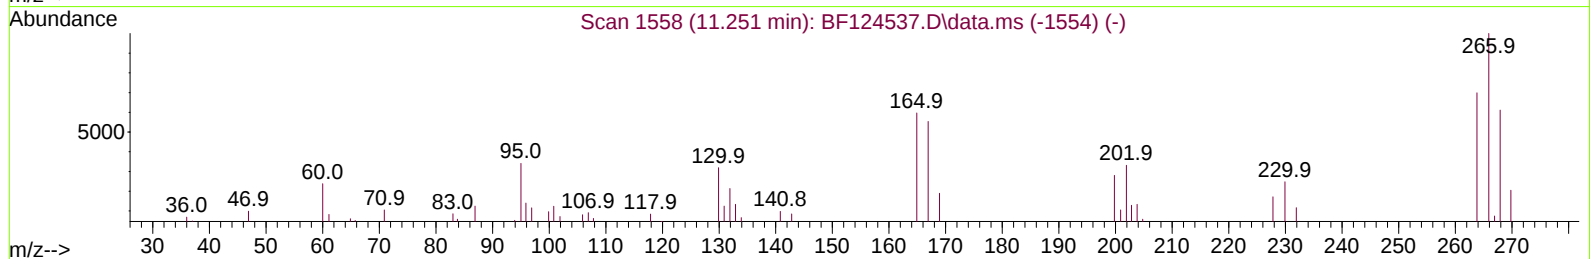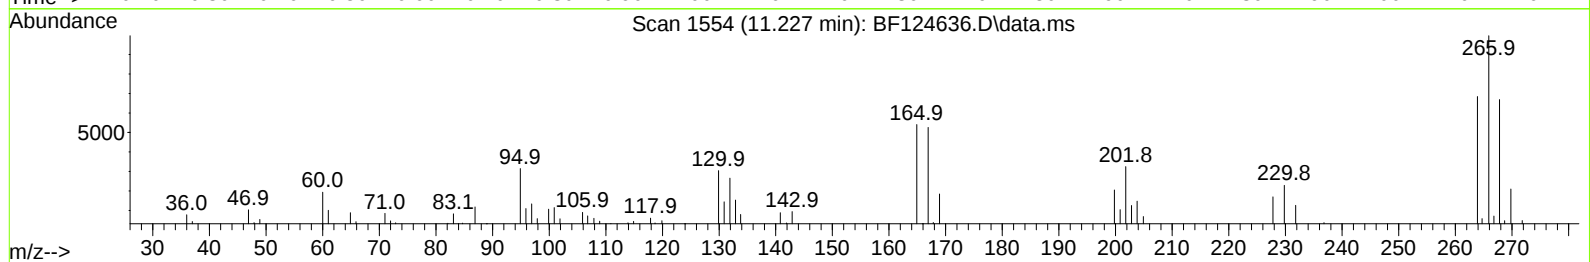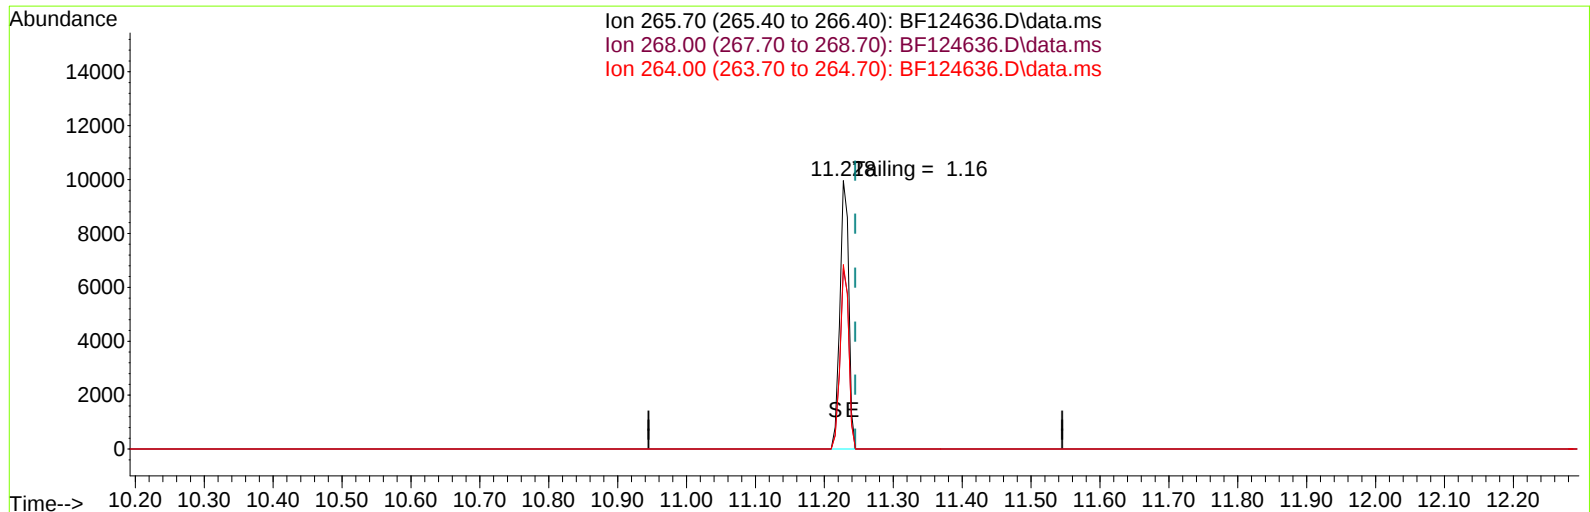

TIC: BF124636.D\data.ms

(70) Pentachlorophenol (C)

11.227min (-0.017) 0.00 ng




response 8912

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	61.10	71.94
264.00	69.90	74.50
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072021\
 Data File : BF124636.D
 Acq On : 20 Jul 2021 19:47
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 21 05:28:56 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF070721.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 20 13:36:28 2021
 Response via : Initial Calibration

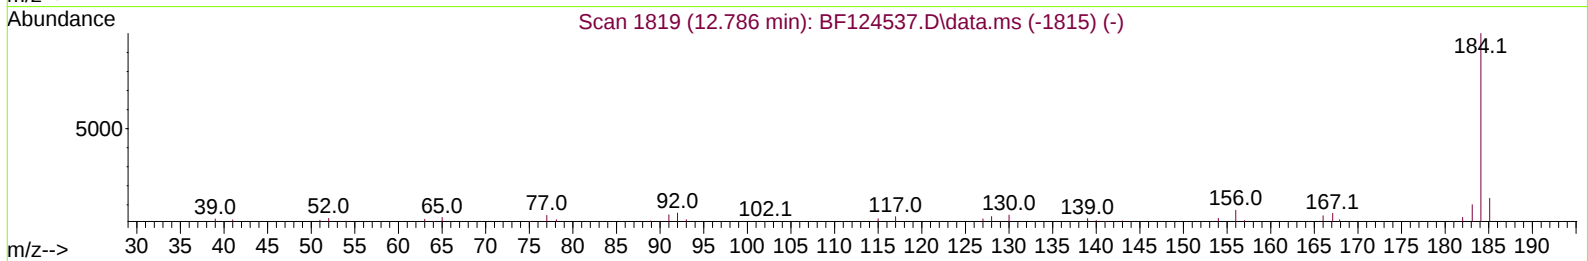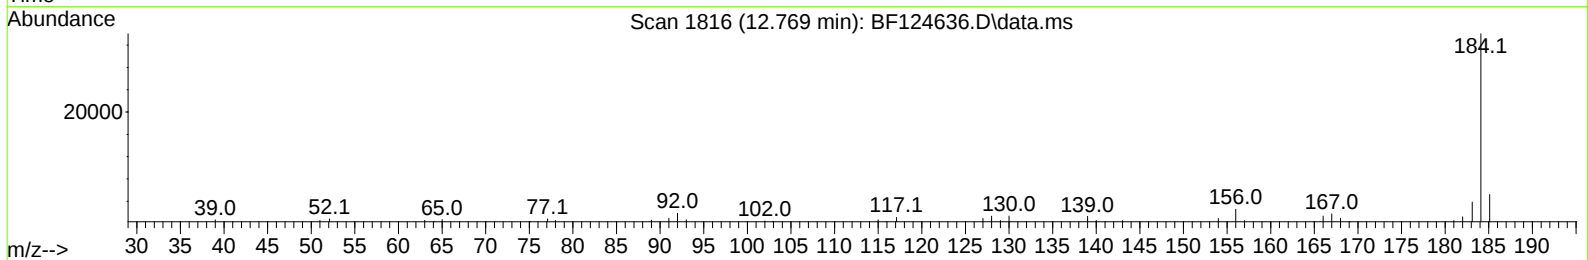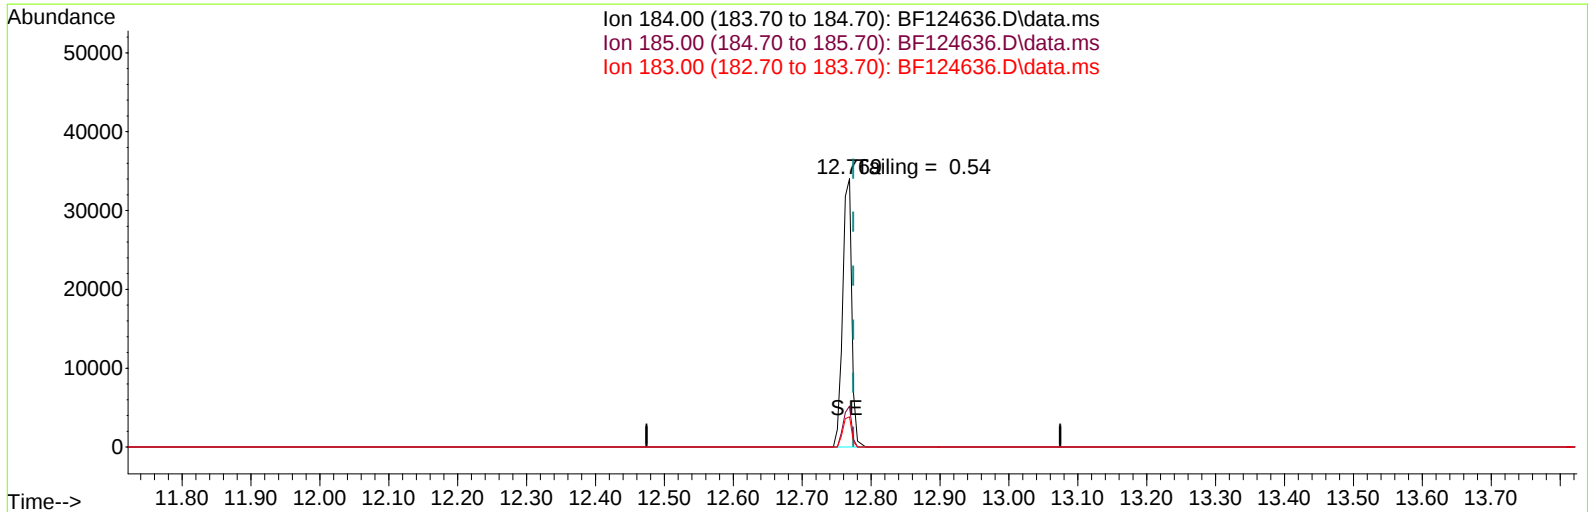

TIC: BF124636.D\data.ms

(77) Benzidine

12.769min (-0.006) 0.00 ng

response 31098

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	13.50	15.27
183.00	10.10	11.30
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/20/2021	BNA_F	BF124636.D
Compound Name	Response	Retention Time
DDT	19637	13.592
DDD	0	13.29
DDE	0	12.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
0	19637	0.00