
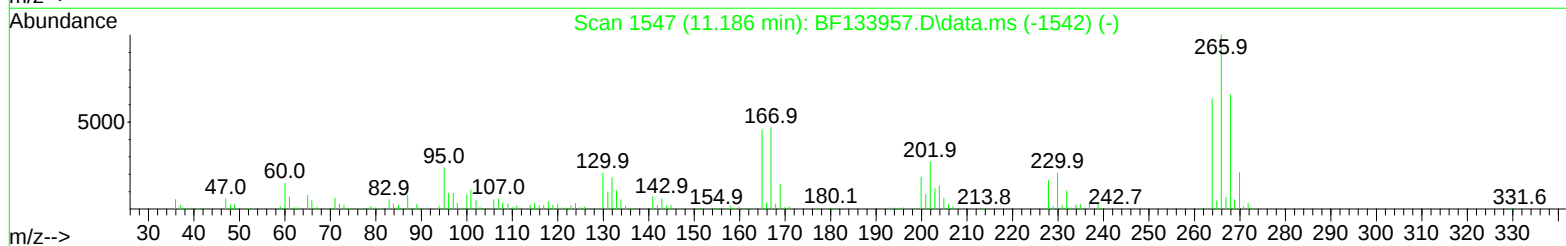
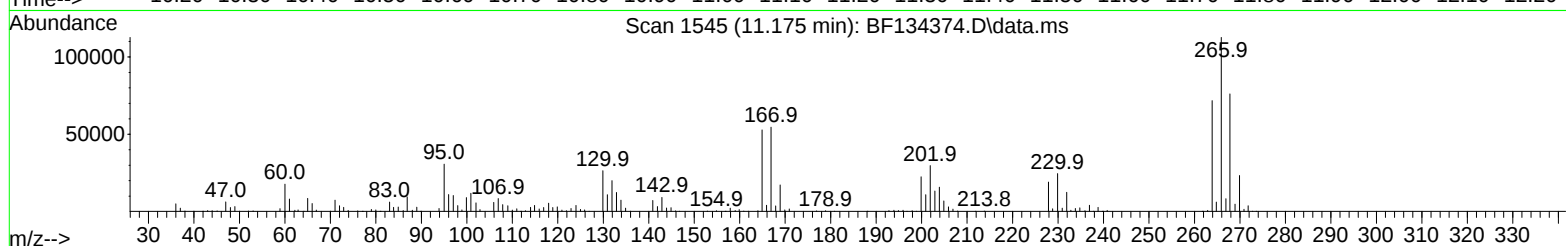


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072023\
Data File : BF134374.D
Acq On : 20 Jul 2023 10:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 13:40:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

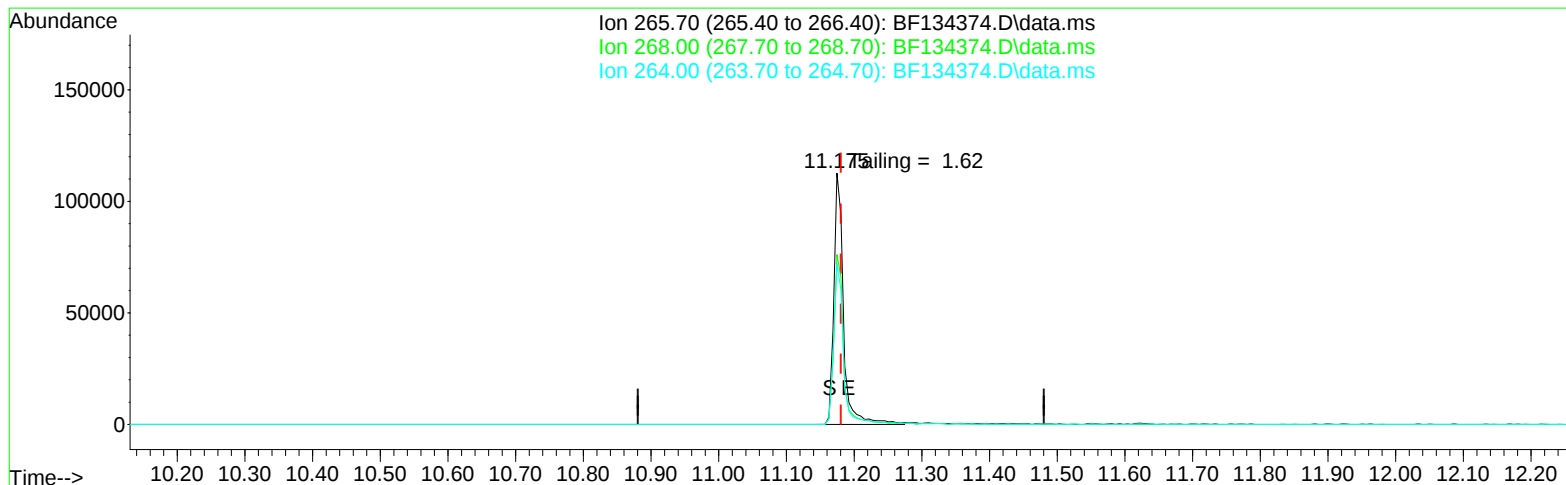

TIC: BF134374.D\data.ms

(70) Pentachlorophenol (C)




11.175min (-0.006) 298769.84 ng

response 110880

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	67.55
264.00	63.30	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072023\
Data File : BF134374.D
Acq On : 20 Jul 2023 10:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 20 13:40:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

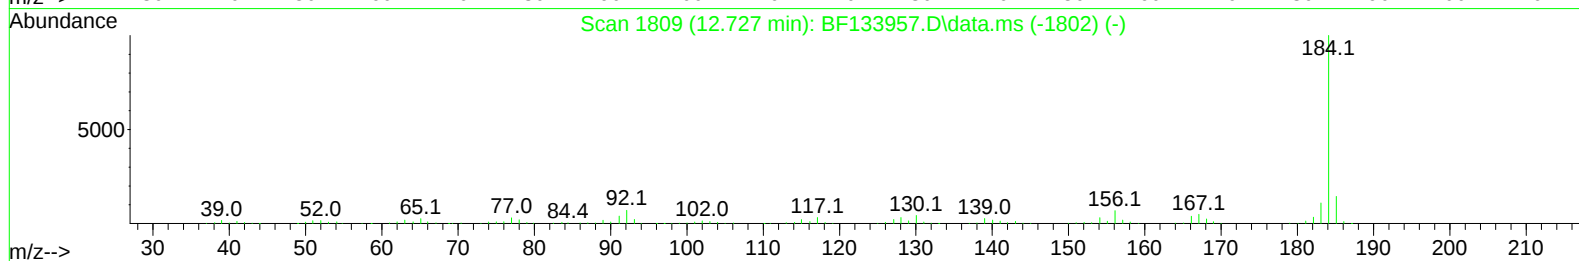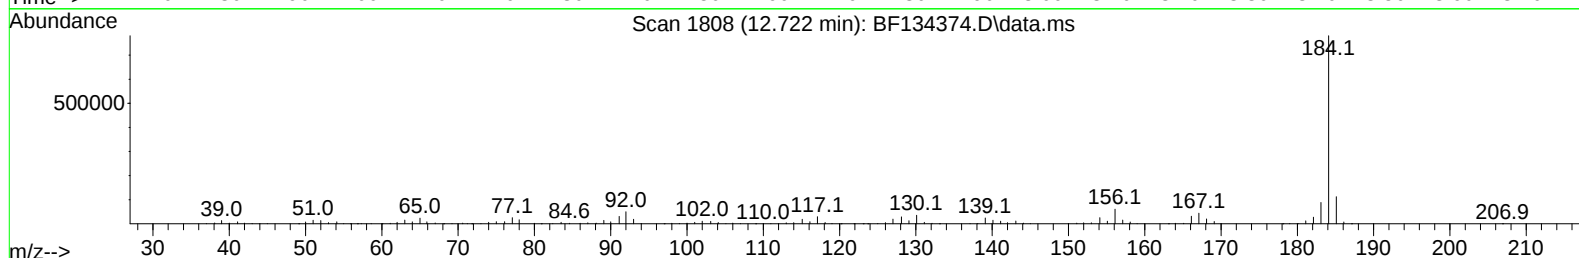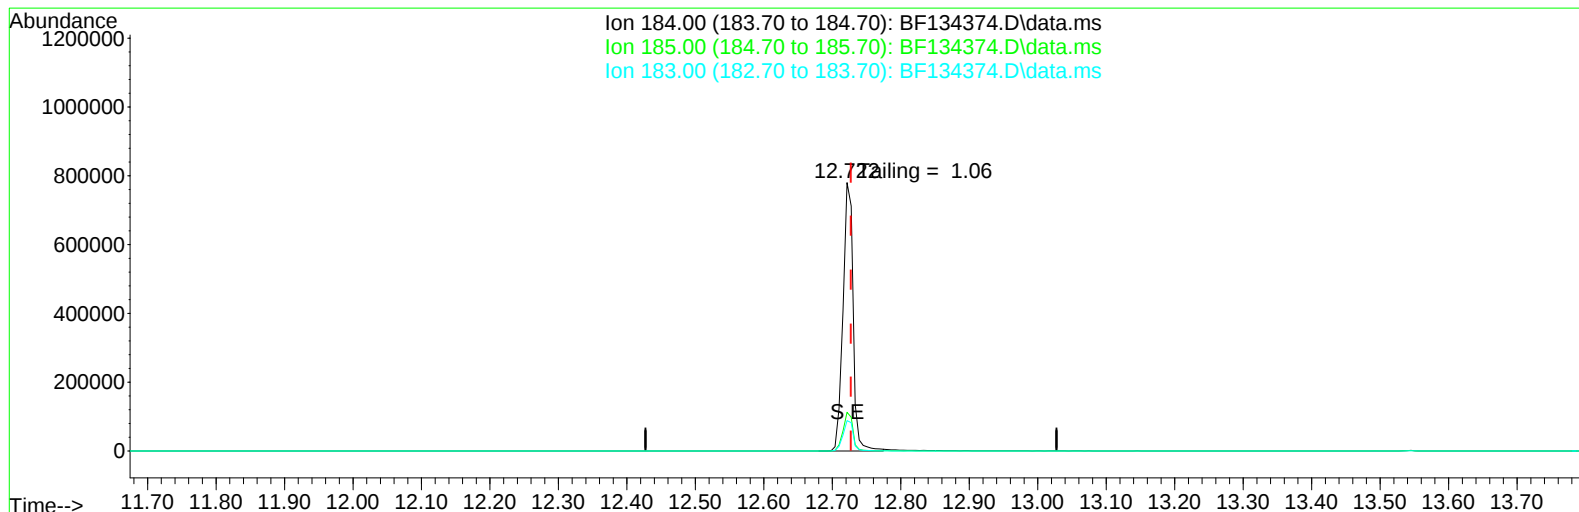

TIC: BF134374.D\data.ms

(77) Benzidine

12.722min (-0.006) 6473.93 ng m

response 802564

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.44
183.00	11.00	11.36
0.00	0.00	0.00