

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072023\
 Data File : BF134376.D
 Acq On : 20 Jul 2023 12:02
 Operator : CG\JU
 Sample : PB154198BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB154198BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134376.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.104	507	513	522	rBV	27169	42676	1.40%	0.256%
2	5.481	573	577	595	rBV	2204741	2269451	74.20%	13.627%
3	6.481	742	747	750	rBV	2086229	2325482	76.03%	13.964%
4	6.834	804	807	817	rBV	488143	444975	14.55%	2.672%
5	7.404	899	904	907	rBV	1481361	1323423	43.27%	7.947%
6	8.116	1021	1025	1040	rBV	585364	481809	15.75%	2.893%
7	9.192	1204	1208	1211	rBV	2795594	2573784	84.15%	15.454%
8	9.875	1320	1324	1327	rBV	664951	548874	17.94%	3.296%
9	10.669	1455	1459	1463	rBV	1832348	1837839	60.09%	11.035%
10	11.369	1574	1578	1586	rBV	737343	617380	20.18%	3.707%
11	12.969	1845	1850	1853	rBV	3185042	3058692	100.00%	18.366%
12	14.033	2027	2031	2040	rBV	570166	569354	18.61%	3.419%
13	15.533	2281	2286	2293	rBV	410553	560228	18.32%	3.364%




Sum of corrected areas: 16653967

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072023\
Data File : BF134376.D
Acq On : 20 Jul 2023 12:02
Operator : CG\JU
Sample : PB154198BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154198BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

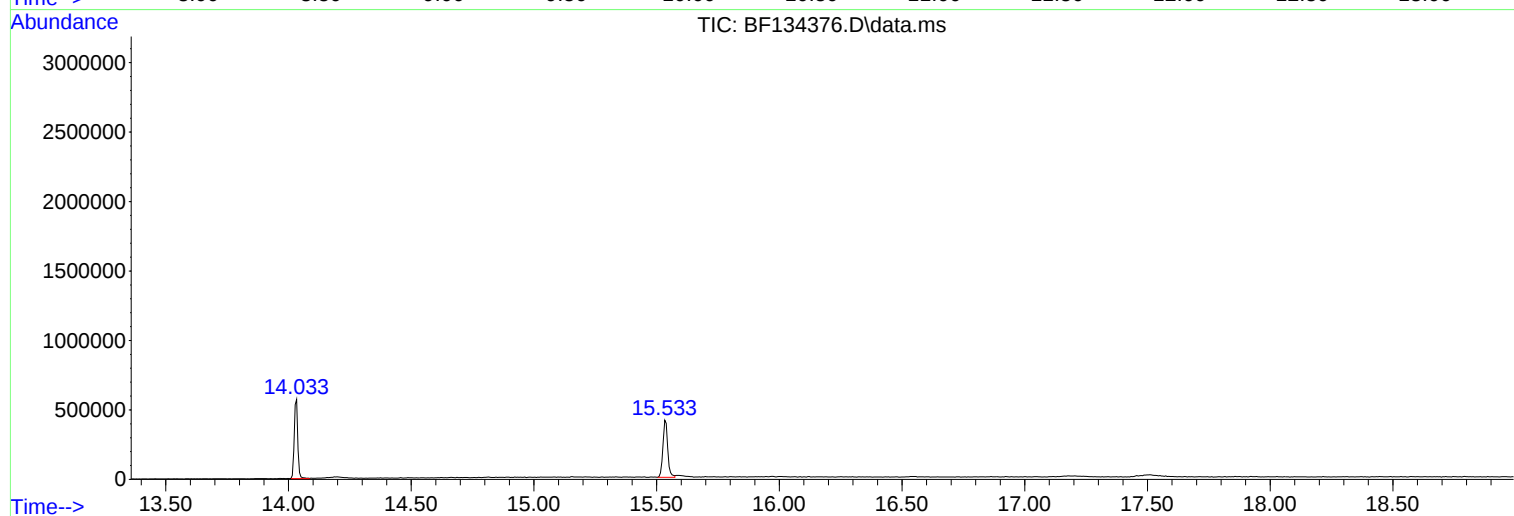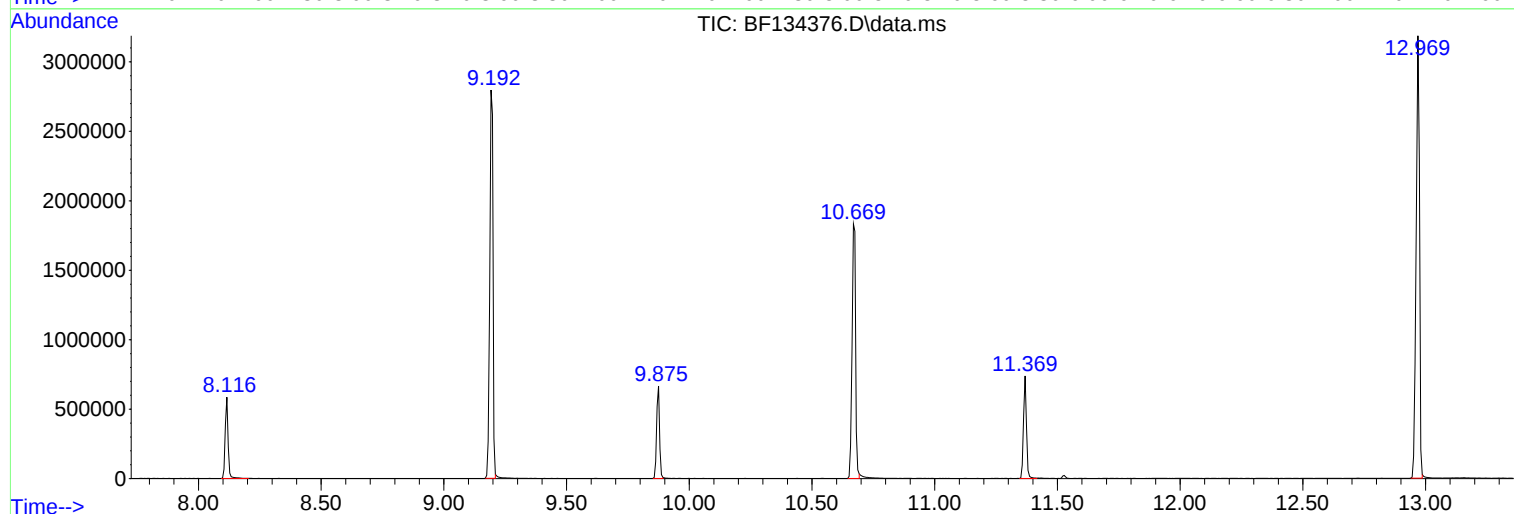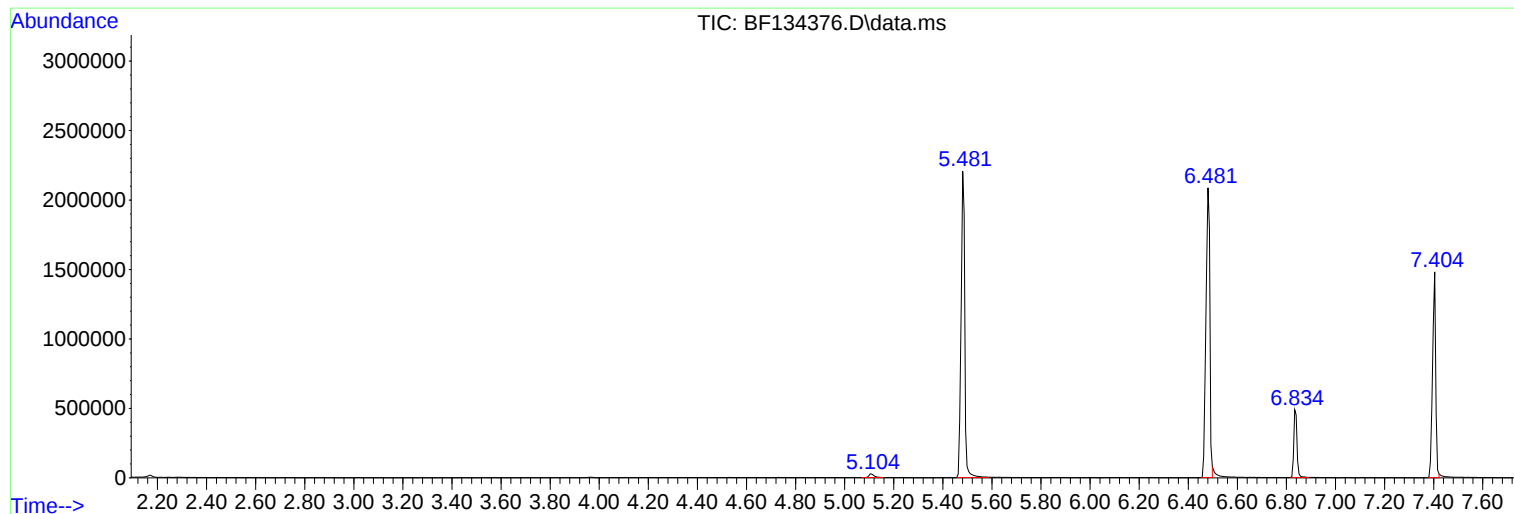

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072023\
Data File : BF134376.D
Acq On : 20 Jul 2023 12:02
Operator : CG\JU
Sample : PB154198BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154198BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072023\
Data File : BF134376.D
Acq On : 20 Jul 2023 12:02
Operator : CG\JU
Sample : PB154198BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154198BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------