
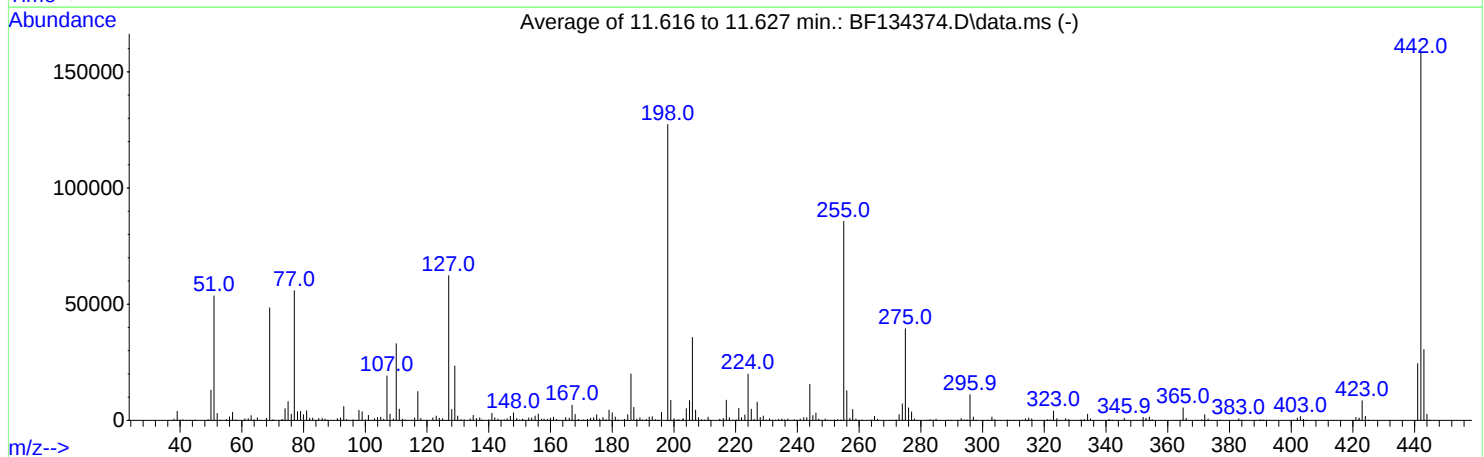


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072023\
Data File : BF134374.D
Acq On : 20 Jul 2023 10:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 14 22:51:27 2023

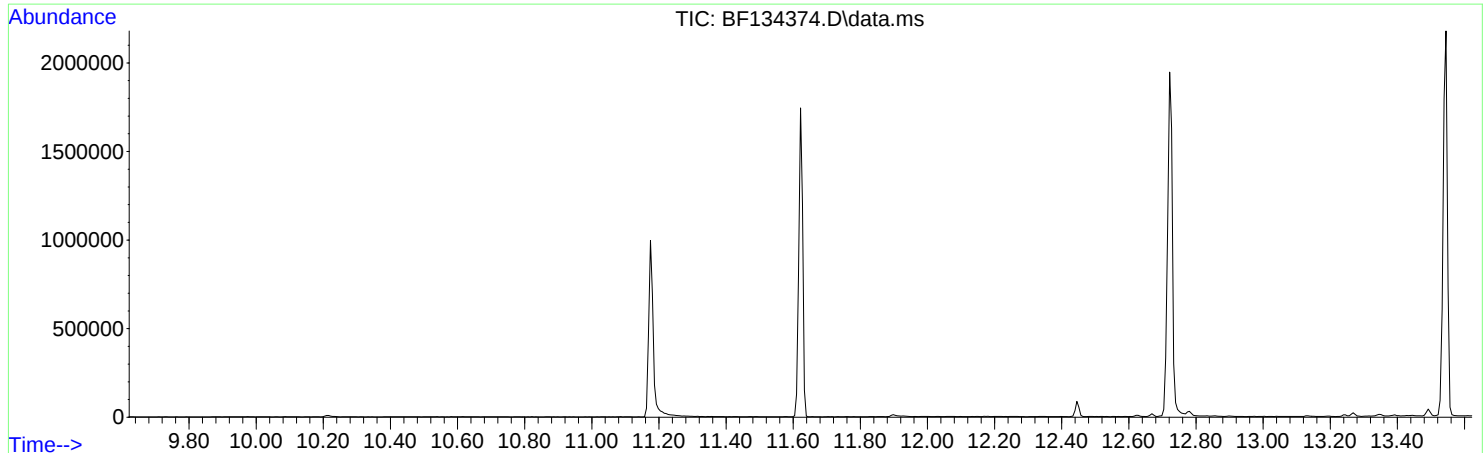




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.1	53576	PASS
68	69	0.00	2	1.9	907	PASS
69	198	0.00	100	38.0	48429	PASS
70	69	0.00	2	0.6	308	PASS
127	198	10	80	48.9	62285	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	127315	PASS
199	198	5	9	6.8	8594	PASS
275	198	10	60	31.0	39432	PASS
365	198	1	100	4.2	5403	PASS
441	198	0.01	100	19.2	24419	PASS
442	442	50	100	100.0	158333	PASS
443	442	15	24	19.3	30481	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072023\
Data File : BF134374.D
Acq On : 20 Jul 2023 10:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 20 13:40:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

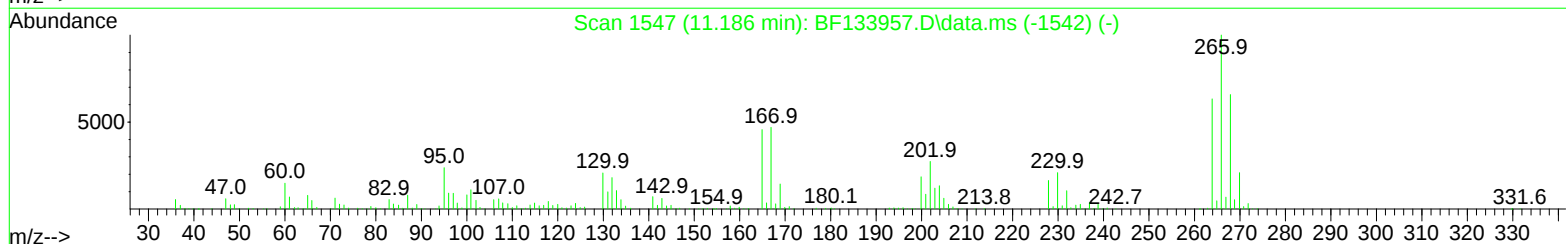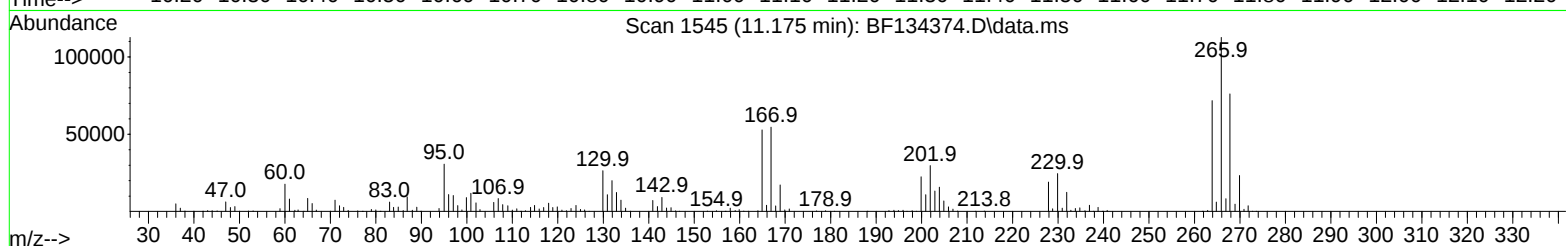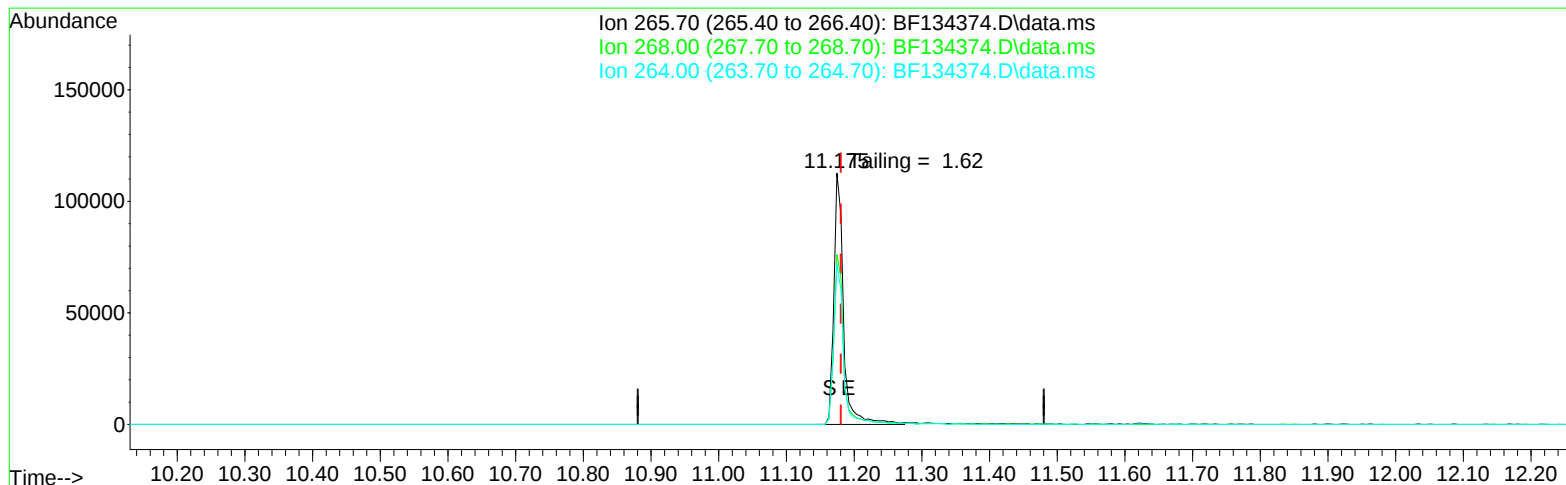

TIC: BF134374.D\data.ms

(70) Pentachlorophenol (C)

11.175min (-0.006) 298769.84 ng




response 110880

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	67.55
264.00	63.30	63.70
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072023\
Data File : BF134374.D
Acq On : 20 Jul 2023 10:56
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 20 13:40:45 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

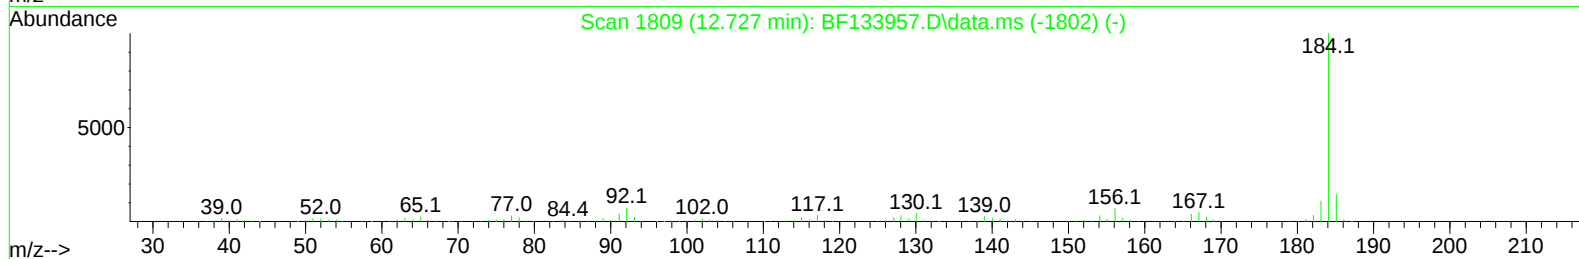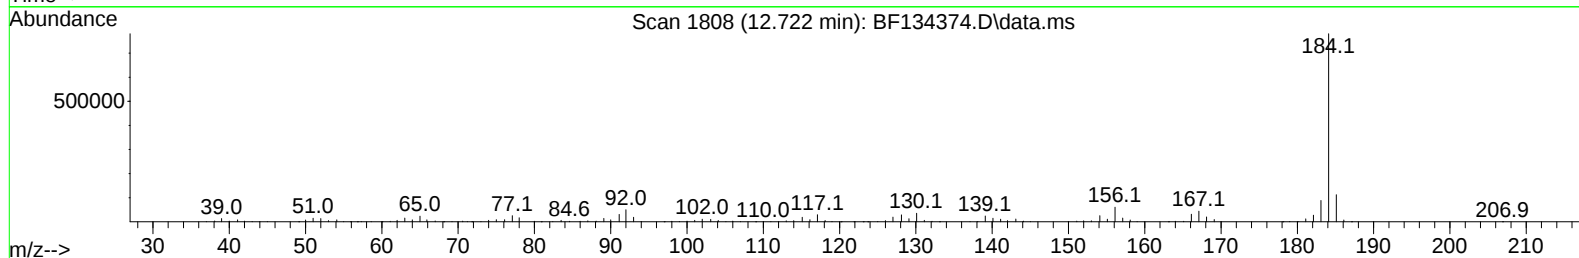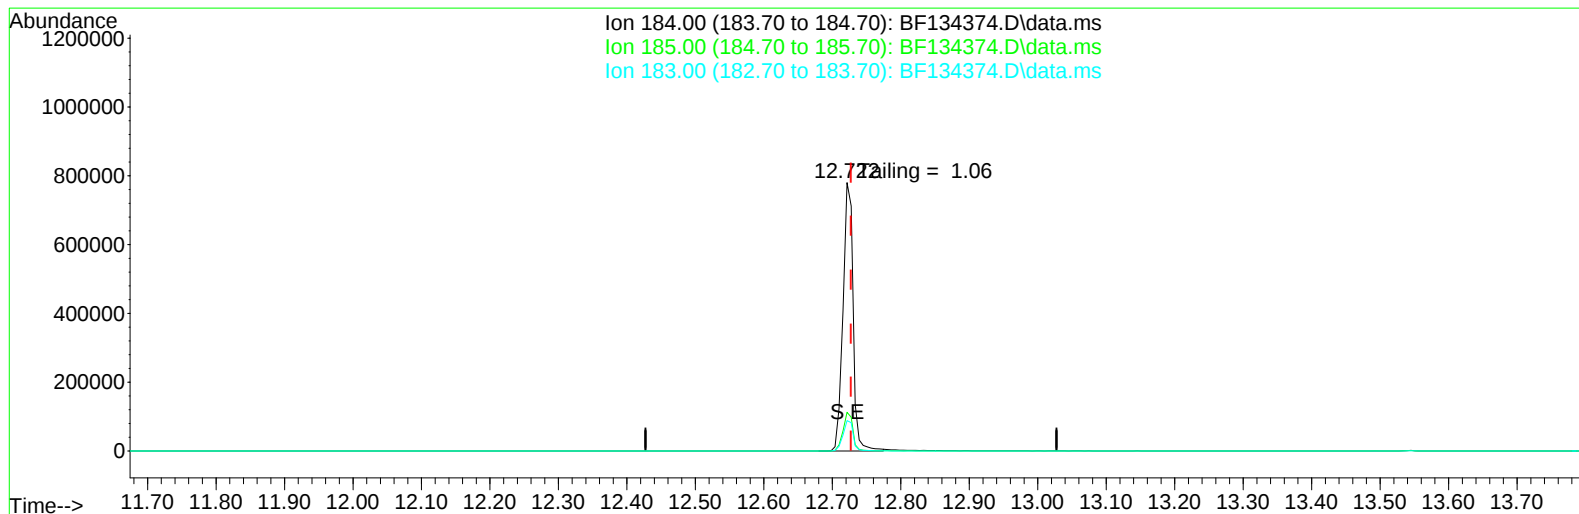

TIC: BF134374.D\data.ms

(77) Benzidine

12.722min (-0.006) 6473.93 ng m

response 802564

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	14.44
183.00	11.00	11.36
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/20/2023	BNA_F	<u>BF134374.D</u>
Compound Name	Response	Retention Time
DDT	381887	13.545
DDD	5709	13.269
DDE	451	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6160	388047	1.59

Instrument :
BNA_F
ClientSampleId :
DFTPP