
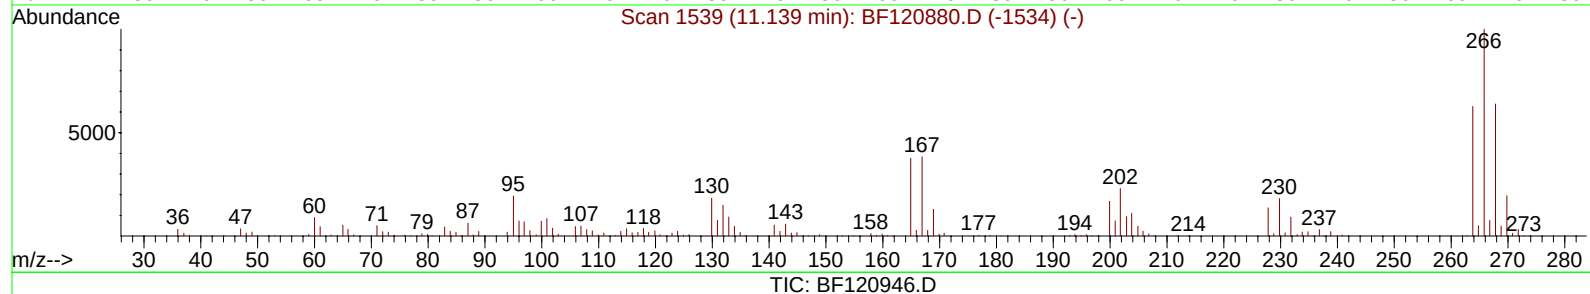
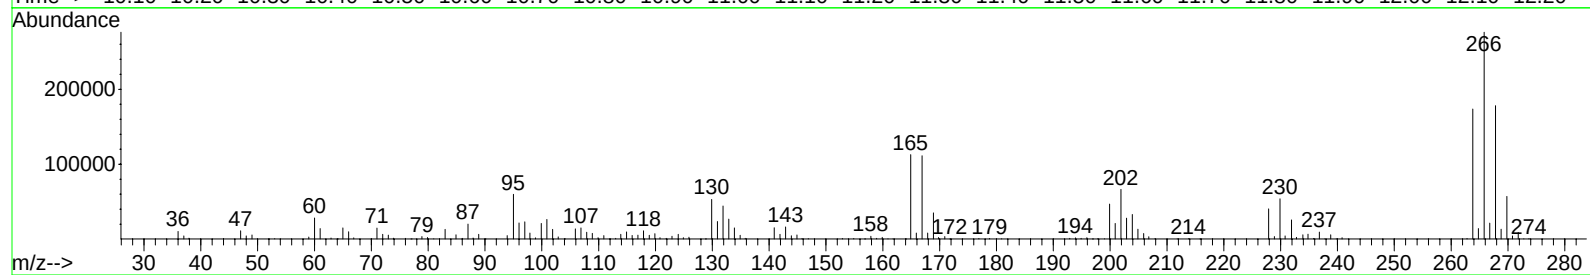


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072120\
 Data File : BF120946.D
 Acq On : 21 Jul 2020 8:30
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 15:59:30 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 16 14:20:32 2020
 Response via : Initial Calibration

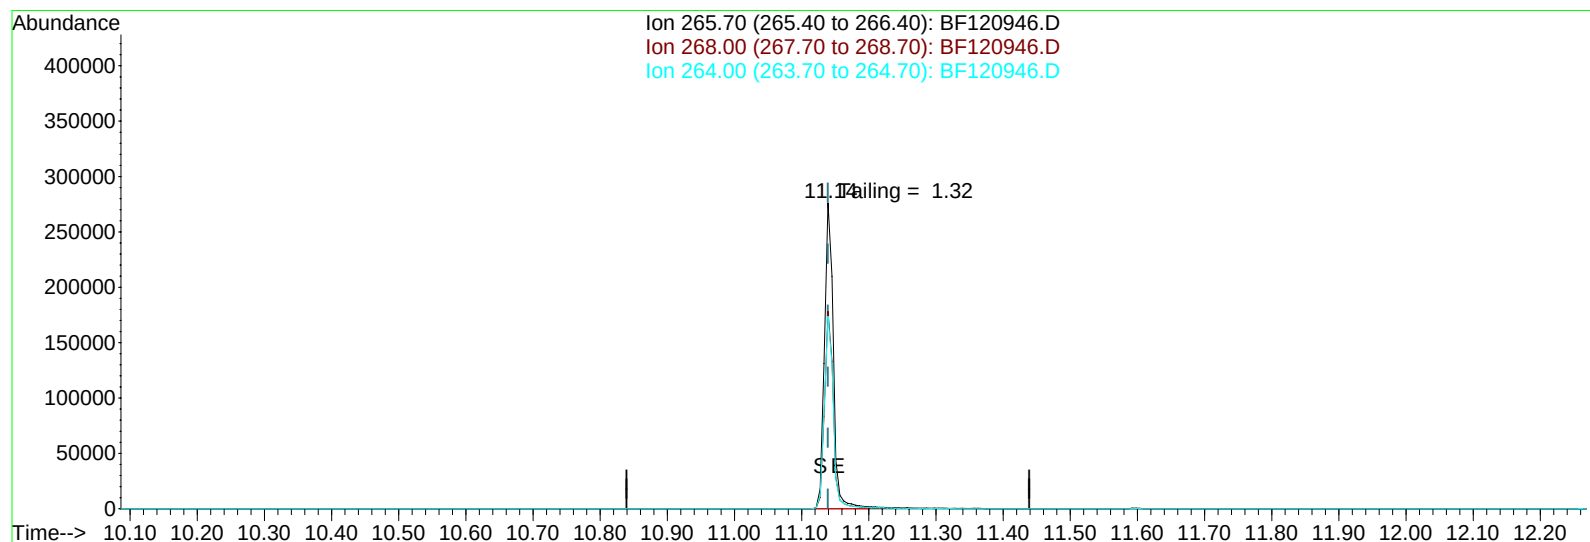

(70) Pentachlorophenol (C)




11.139min (+0.000) 121667.28ng

response 258075

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.53
264.00	62.70	62.89
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072120\
Data File : BF120946.D
Acq On : 21 Jul 2020 8:30
Operator : JU/CG
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 15:59:30 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 16 14:20:32 2020
Response via : Initial Calibration

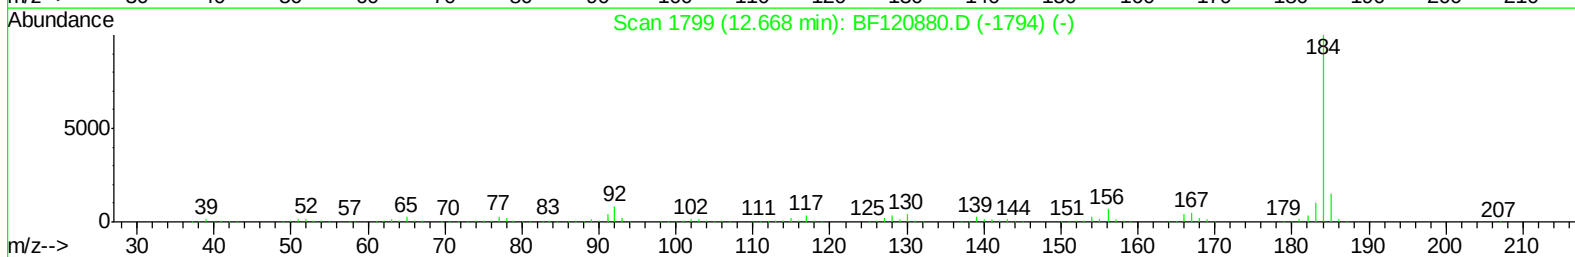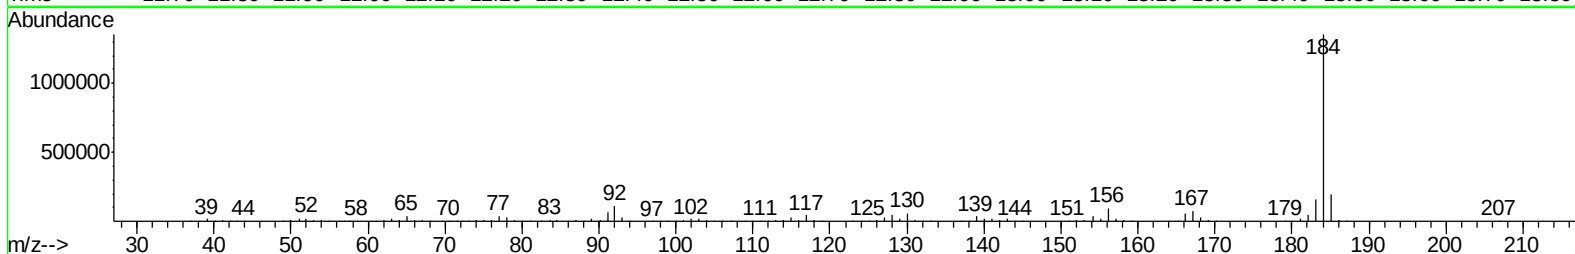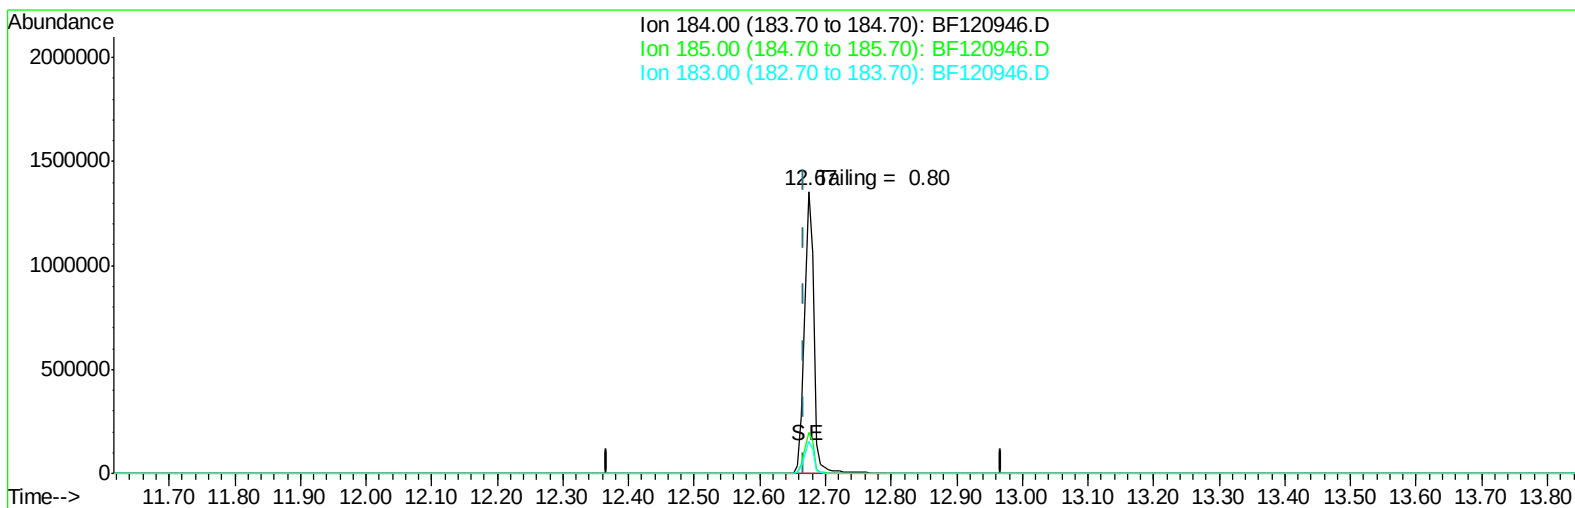

TIC: BF120946.D

(77) Benzidine

12.674min (+0.006) 146577.36ng

response 1371946

Ion	Exp%	Act%
184.00	100	100
185.00	15.20	14.76
183.00	10.60	11.39
0.00	0.00	0.00