

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072120\
 Data File : BF120951.D
 Acq On : 21 Jul 2020 12:47
 Operator : JU/CG
 Sample : PB130338BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130338BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.163	9	13	19	rVB	78663	110531	1.92%	0.291%
2	5.440	565	570	573	rBV	3859149	4614917	80.10%	12.140%
3	6.446	735	741	744	rBV	3568117	4578325	79.46%	12.044%
4	6.810	799	803	807	rBV	1422681	1169341	20.30%	3.076%
5	7.375	893	899	902	rBV	2760791	3155120	54.76%	8.300%
6	8.092	1016	1021	1025	rBV	1470457	1557400	27.03%	4.097%
7	9.175	1198	1205	1208	rBV	4366293	5639827	97.89%	14.836%
8	9.851	1314	1320	1323	rBV	1564795	1788817	31.05%	4.706%
9	10.639	1447	1454	1481	rBV	2900951	3728603	64.71%	9.808%
10	11.333	1566	1572	1579	rBV	2053871	1927638	33.46%	5.071%
11	12.927	1835	1843	1846	rBV	4679350	5761647	100.00%	15.156%
12	13.763	1979	1985	1988	rBV	44471	71131	1.23%	0.187%
13	13.798	1988	1991	1994	rVV	53627	72466	1.26%	0.191%
14	13.845	1994	1999	2003	rVB	135550	187463	3.25%	0.493%
15	13.969	2016	2020	2031	rVB	1931937	1857900	32.25%	4.887%
16	15.421	2261	2267	2289	rBV	1209678	1793365	31.13%	4.718%


Sum of corrected areas: 38014491

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072120\
Data File : BF120951.D
Acq On : 21 Jul 2020 12:47
Operator : JU/CG
Sample : PB130338BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130338BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

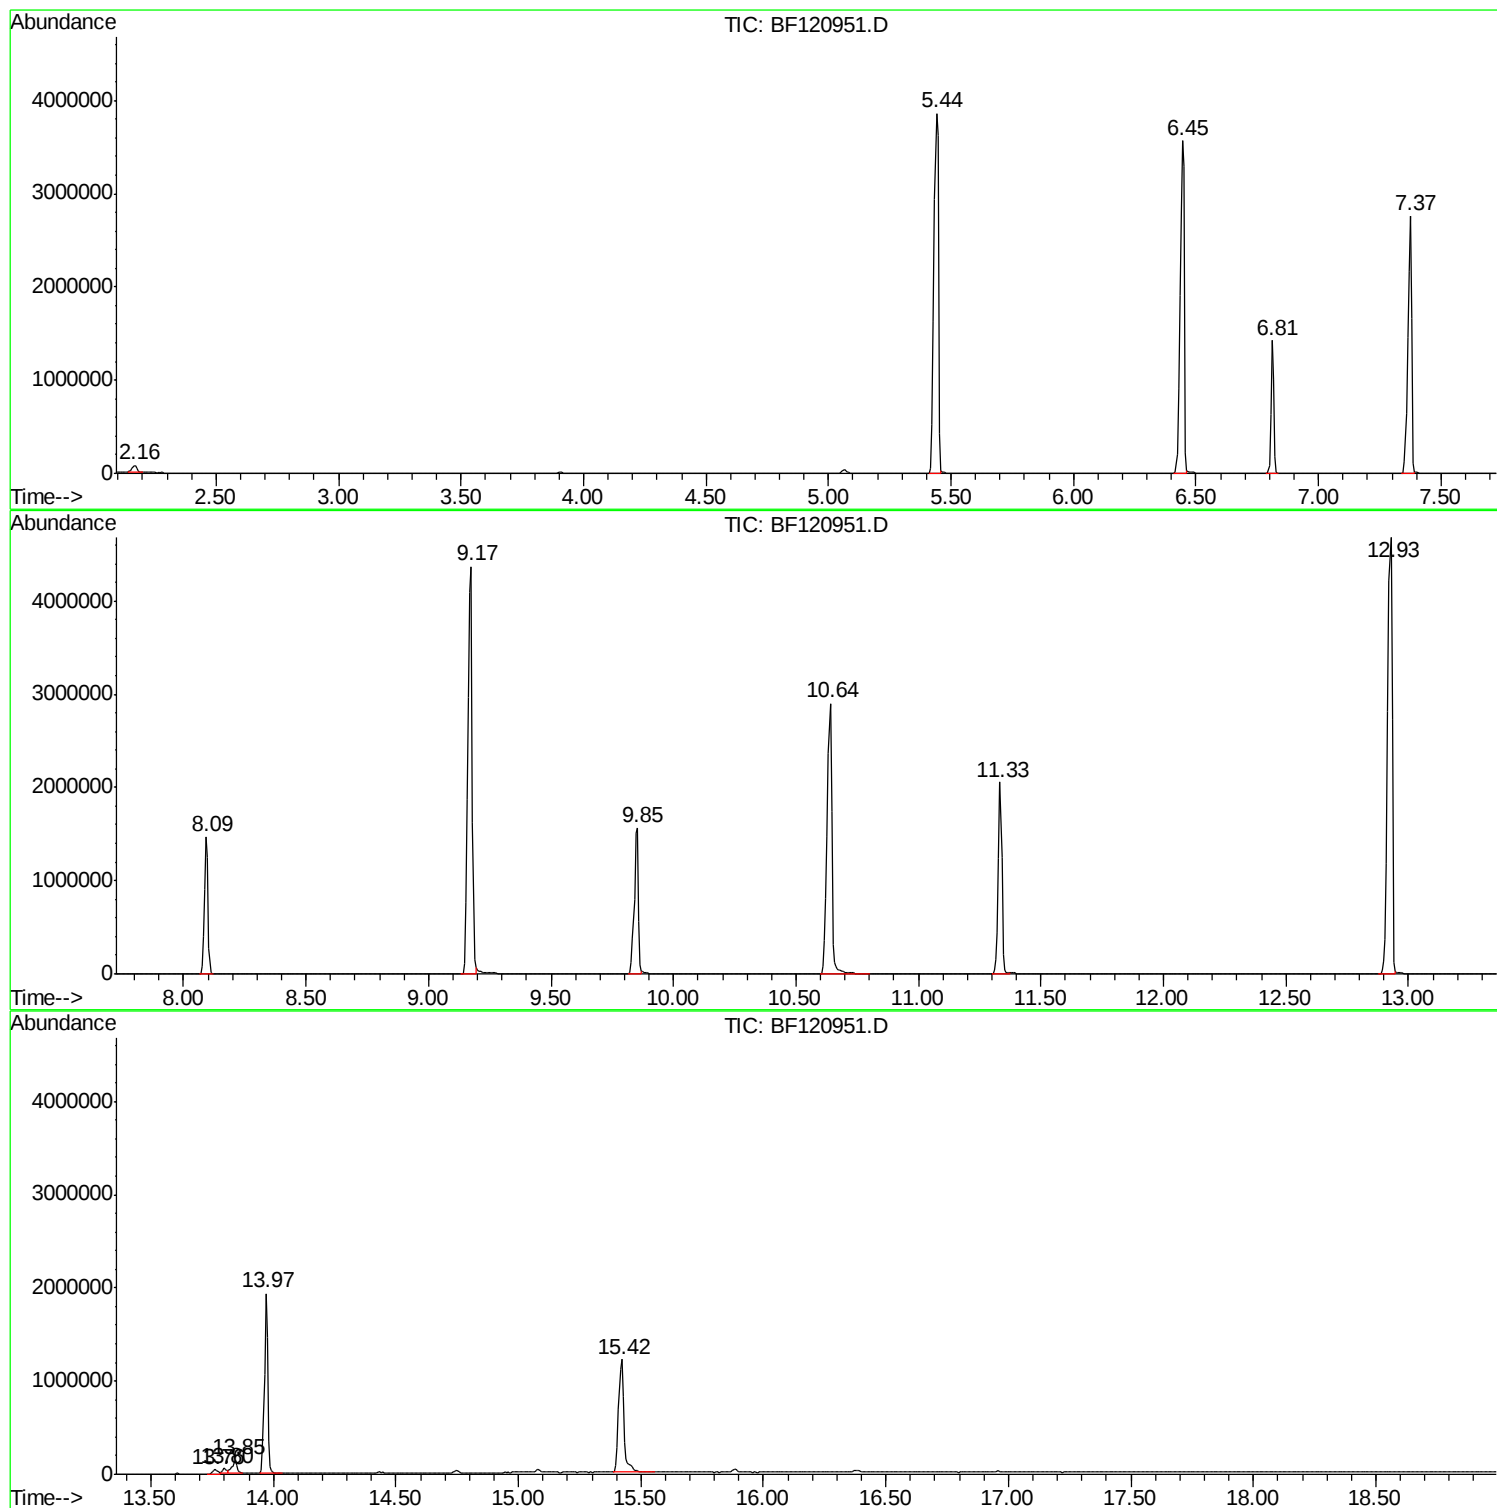

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072120\
Data File : BF120951.D
Acq On : 21 Jul 2020 12:47
Operator : JU/CG
Sample : PB130338BL
Misc :
ALS Vial : 6 Sample Multiplier: 1










Instrument :
BNA_F
ClientSampleId :
PB130338BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Diethylene glycol dibenzoate Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD		R.T.		
13.85	2.02 ng	187463	Chrysene-d12		13.97		
Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Diethylene glycol dibenzoate	314	C18H18O5	000120-55-8	90
2			2,2'-(Ethane-1,2-diylbis(oxv))bi...	358	C20H22O6	1000366-99-4	74
3			2-(2-(2-Methoxvethoxv)ethoxv)eth...	268	C14H20O5	1000366-99-1	74
4			2,5,8,11-Tetraoxatridecan-13-yl ...	312	C16H24O6	1000366-96-7	74
5			3,6,9,12-Tetraoxatetradecane-1,1...	446	C24H30O8	1000366-97-0	72

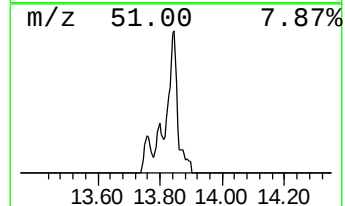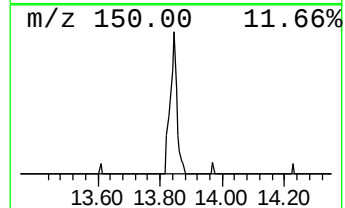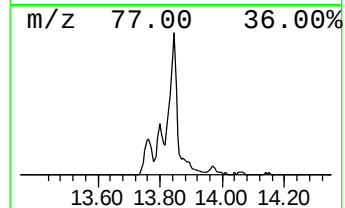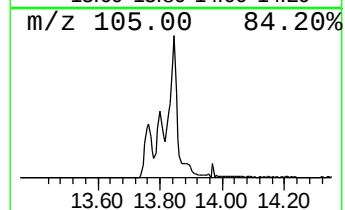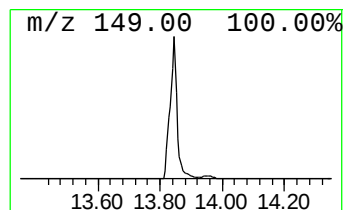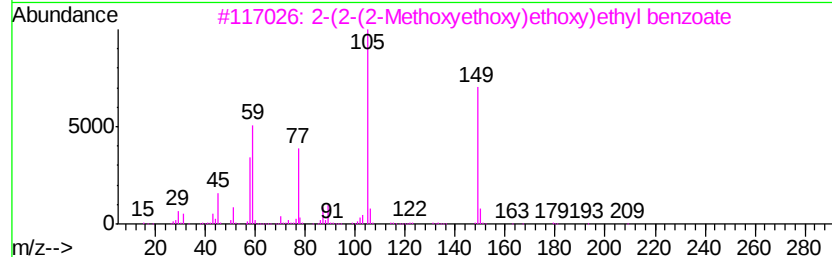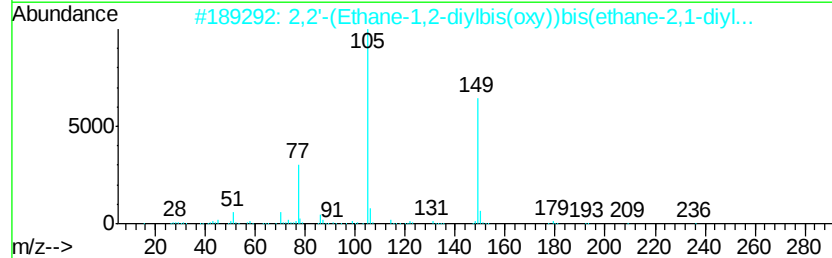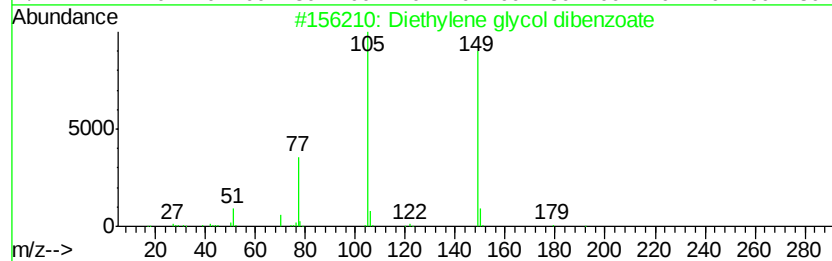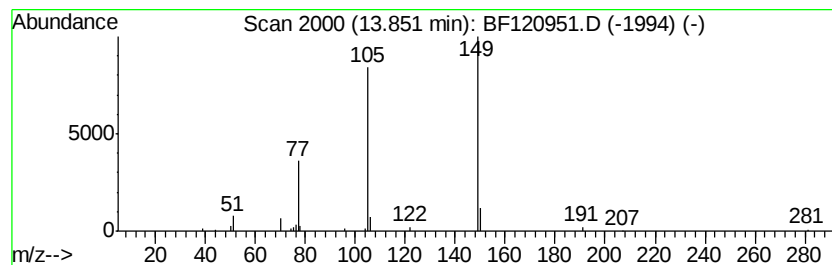

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072120\
Data File : BF120951.D
Acq On : 21 Jul 2020 12:47
Operator : JU/CG
Sample : PB130338BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130338BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Diethylene glycol...	13.85	2.0	ng	187463	5	13.97	1857900	20.0