


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072120\
 Data File : BF120946.D
 Acq On : 21 Jul 2020 8:30
 Operator : JU/CG
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 16 14:20:32 2020

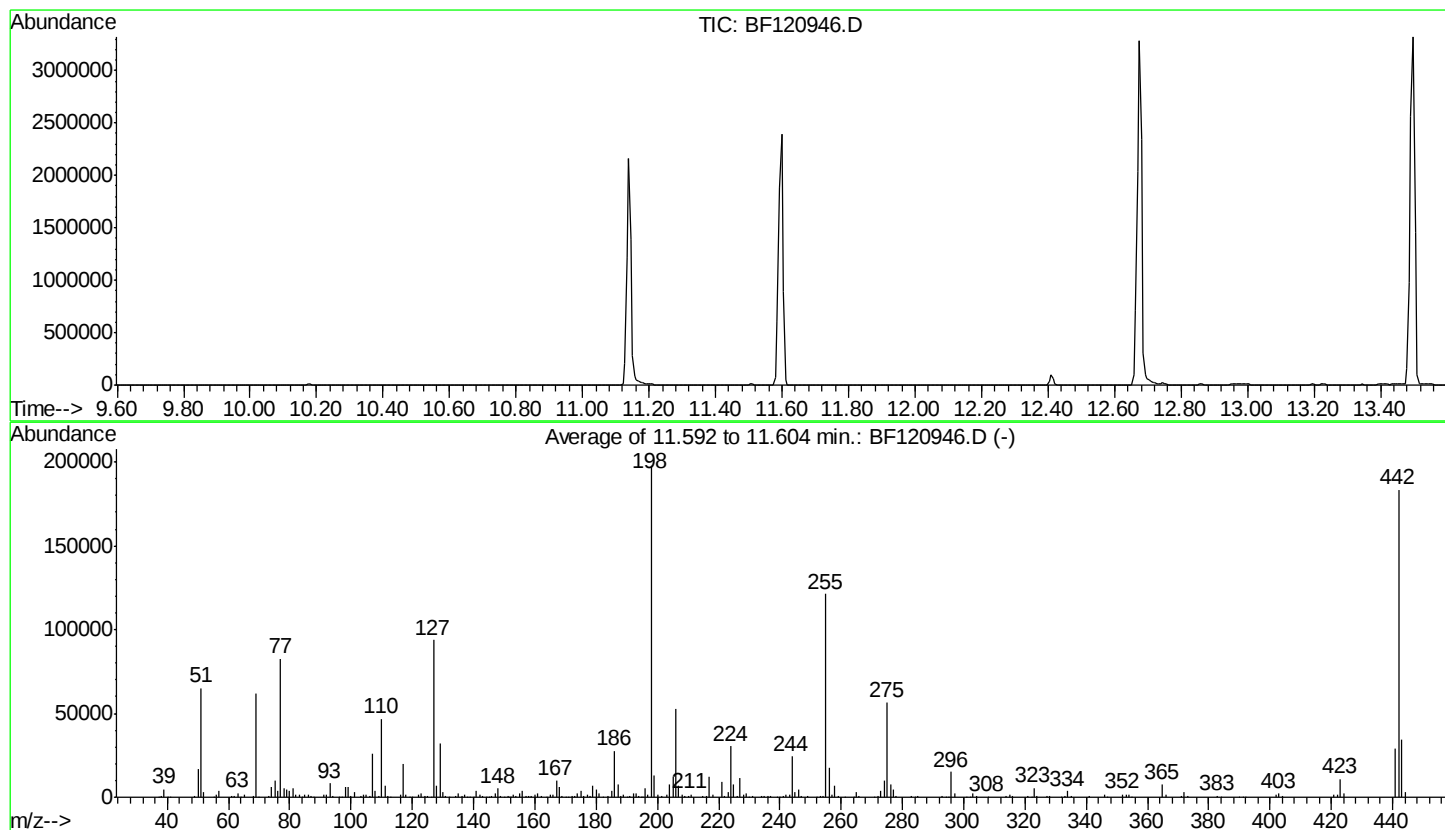

AutoFind: Scans 1616, 1617, 1618; Background Corrected with Scan 1610

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.0	65221	PASS
68	69	0.00	2	1.8	1086	PASS
69	198	0.00	100	31.2	61714	PASS
70	69	0.00	2	0.5	304	PASS
127	198	10	80	47.4	93826	PASS
197	198	0.00	2	0.7	1353	PASS
198	198	100	100	100.0	197853	PASS
199	198	5	9	6.7	13332	PASS
275	198	10	60	28.5	56426	PASS
365	198	1	100	3.8	7600	PASS
441	198	0.01	100	14.6	28896	PASS
442	198	50	100	92.8	183624	PASS
443	442	15	24	18.9	34773	PASS