
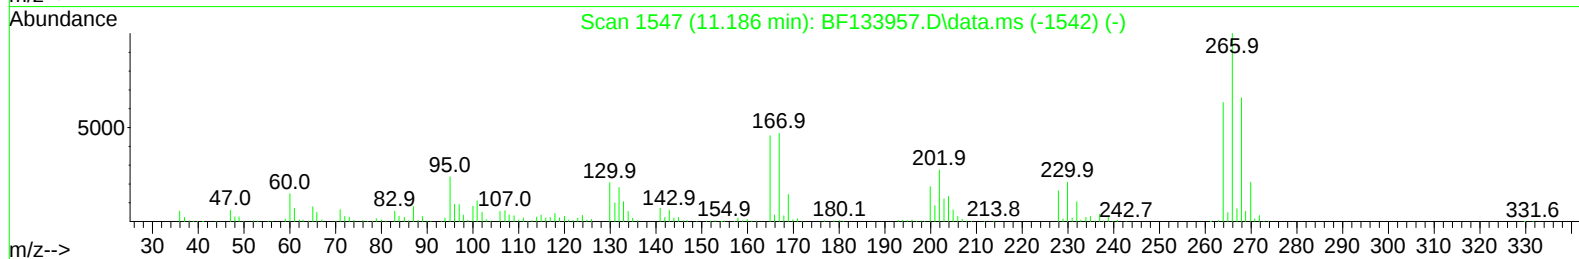
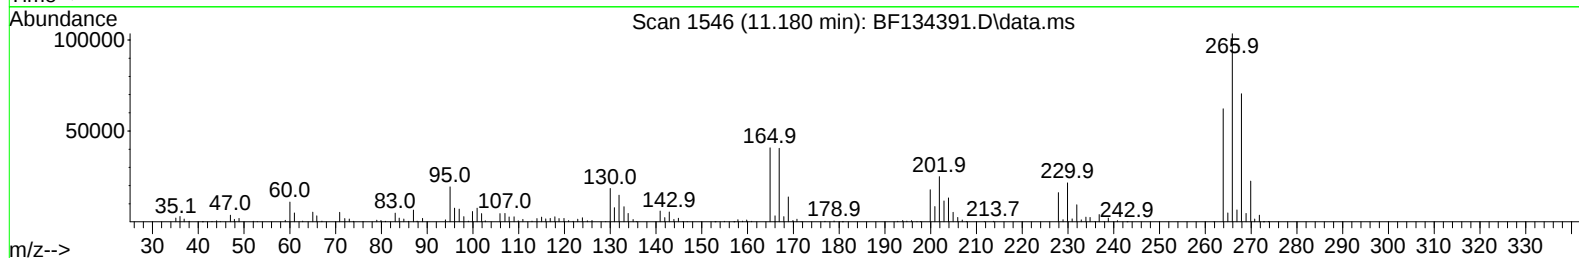


Quant Time: Jul 21 13:25:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

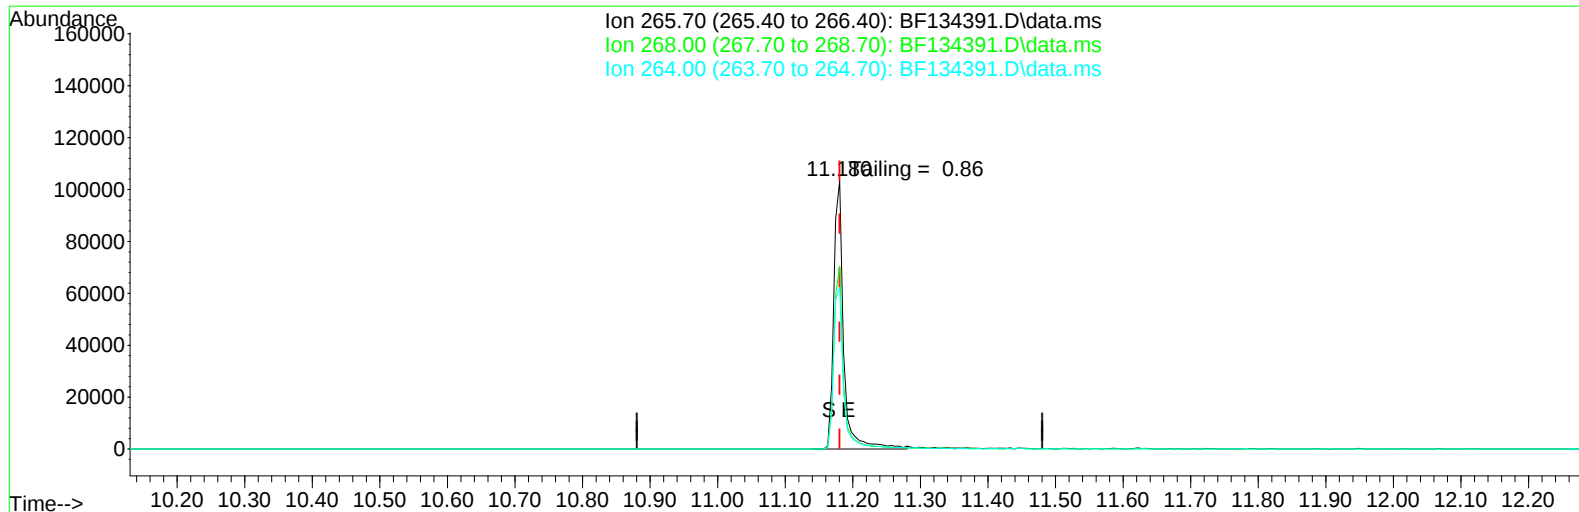

TIC: BF134391.D\data.ms

11.180min (+ 0.000) 29795.98 ng

response **105352**

Ion	Exp%	Act%
-----	------	------

265.70	100.00	100.00
--------	--------	--------




268.00	65.80	68.15
--------	-------	-------

264.00	63.30	60.16
--------	-------	-------

0.00 0.00 0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072123\
 Data File : BF134391.D
 Acq On : 21 Jul 2023 09:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 21 13:25:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 14 22:51:27 2023
 Response via : Initial Calibration

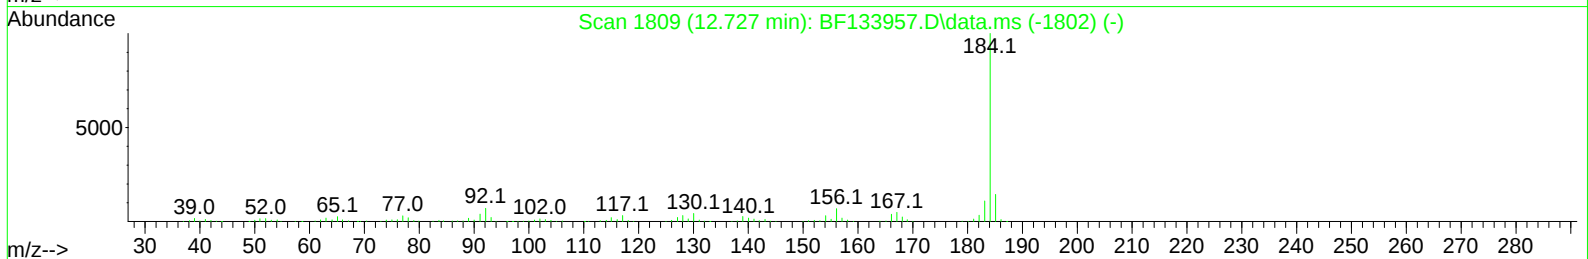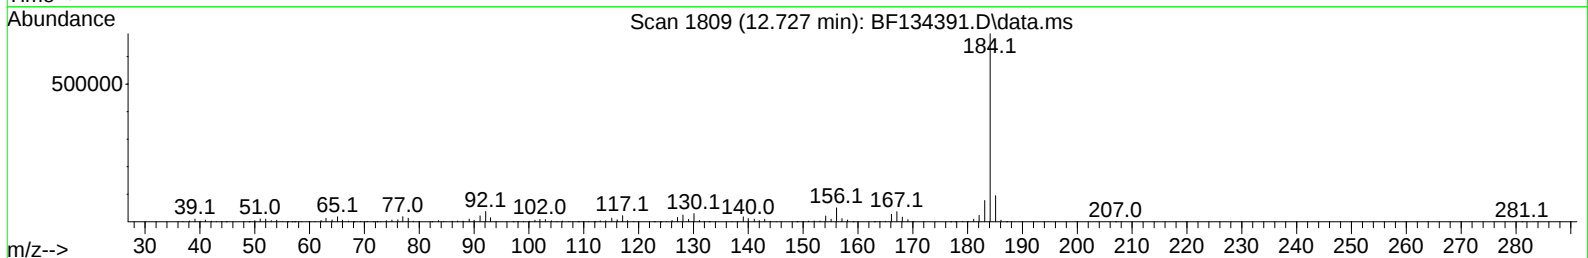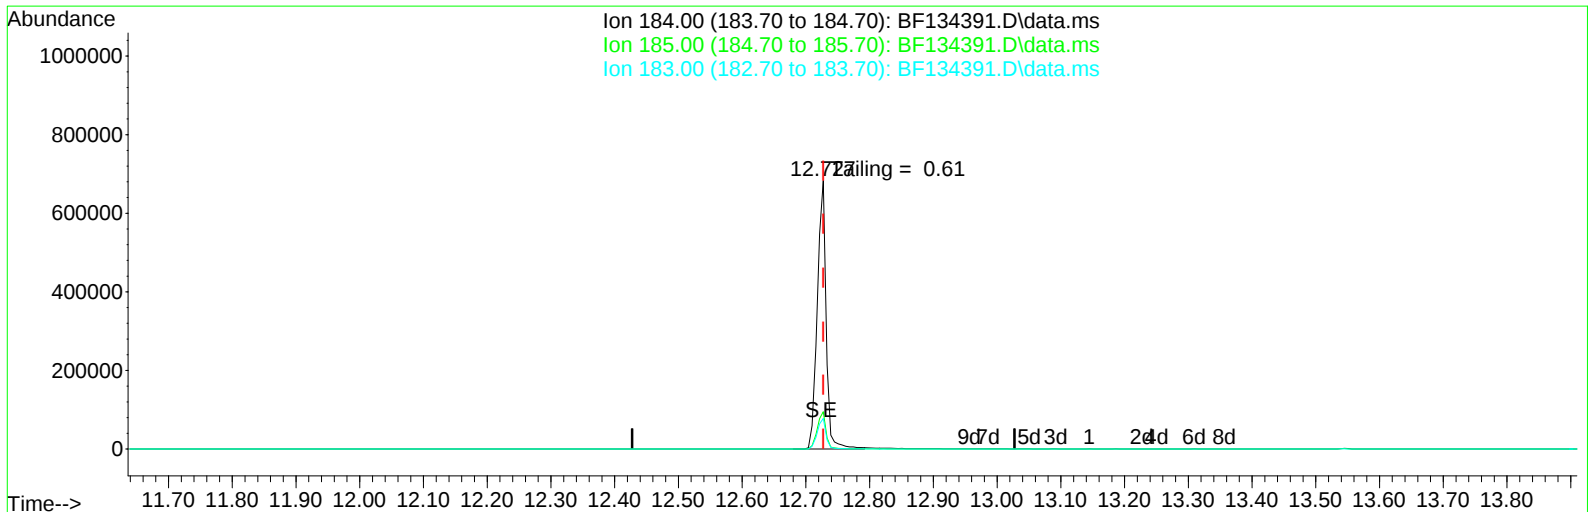

TIC: BF134391.D\data.ms

(77) Benzidine

12.727min (+ 0.000) 512030.47 ng m

response 657905

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.92
183.00	11.00	11.38
0.00	0.00	0.00