


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072123\
Data File : BF134391.D
Acq On : 21 Jul 2023 09:26
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 14 22:51:27 2023

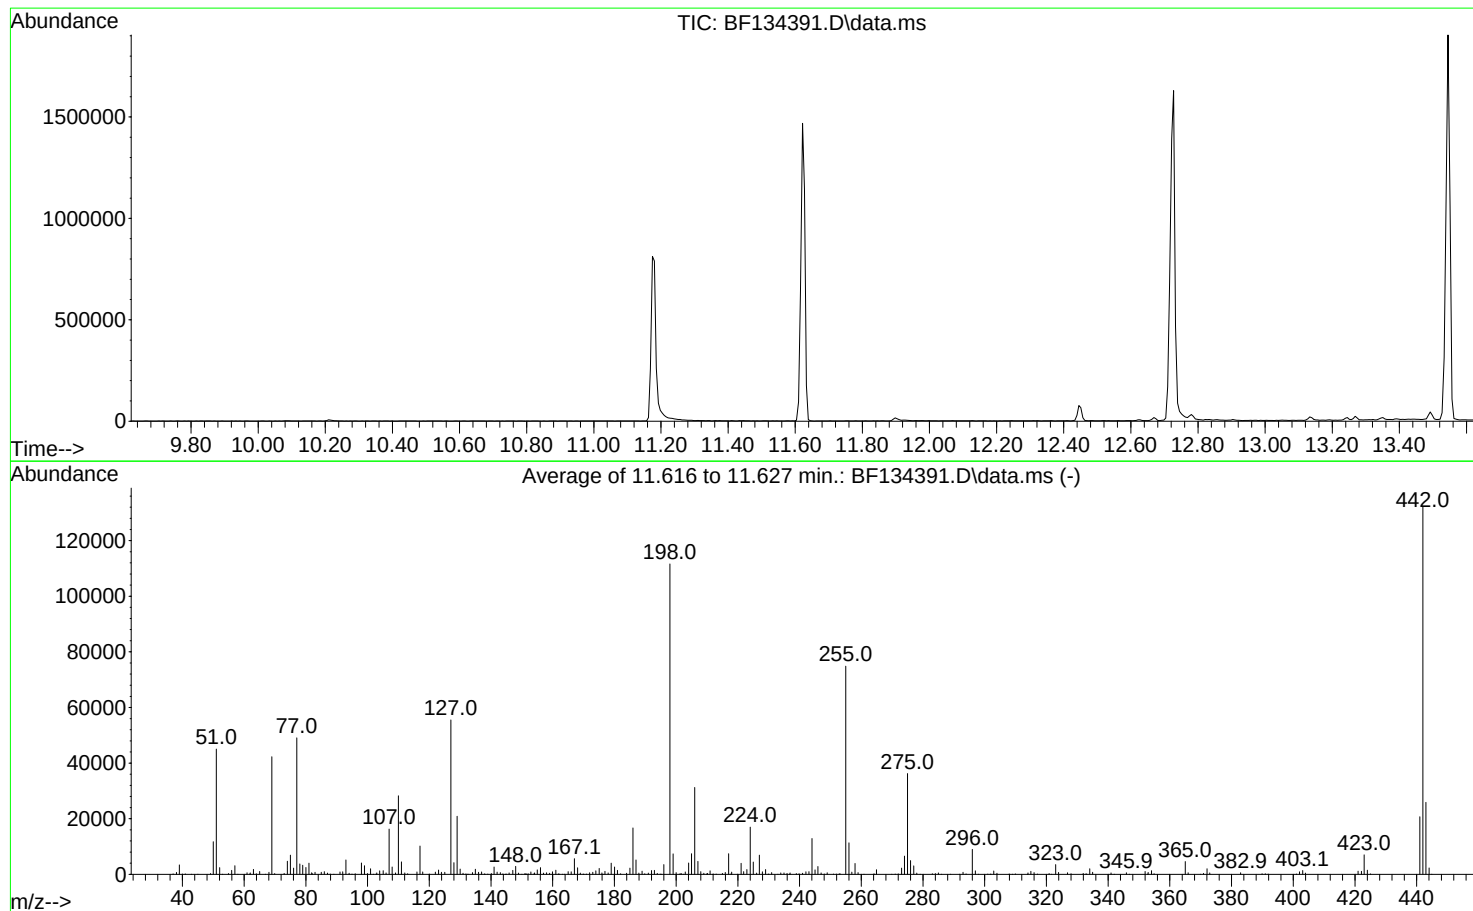




AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.3	45029	PASS
68	69	0.00	2	1.7	740	PASS
69	198	0.00	100	37.9	42304	PASS
70	69	0.00	2	0.8	319	PASS
127	198	10	80	49.7	55507	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	111605	PASS
199	198	5	9	6.6	7349	PASS
275	198	10	60	32.5	36227	PASS
365	198	1	100	4.1	4597	PASS
441	198	0.01	100	18.6	20717	PASS
442	442	50	100	100.0	132264	PASS
443	442	15	24	19.6	25916	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072123\
 Data File : BF134391.D
 Acq On : 21 Jul 2023 09:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 21 13:25:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 14 22:51:27 2023
 Response via : Initial Calibration

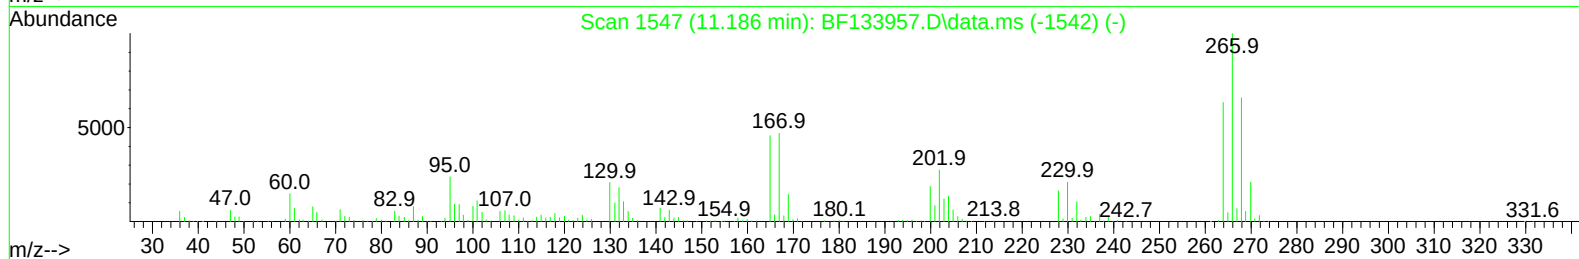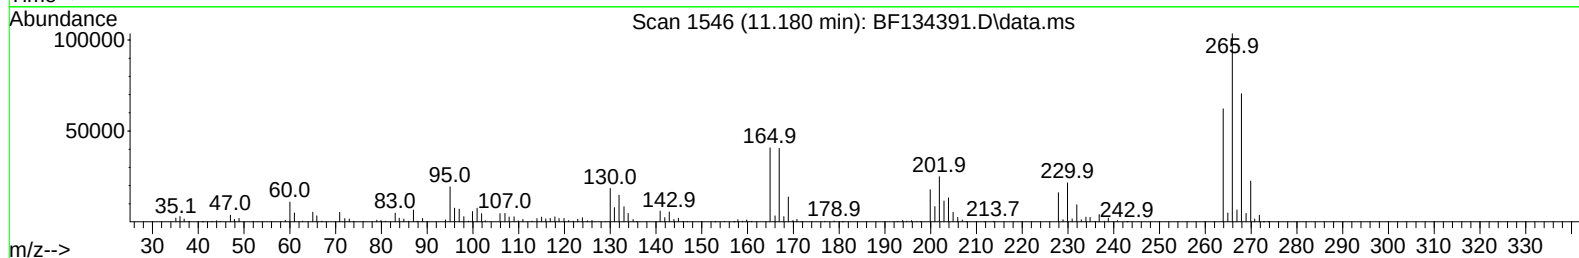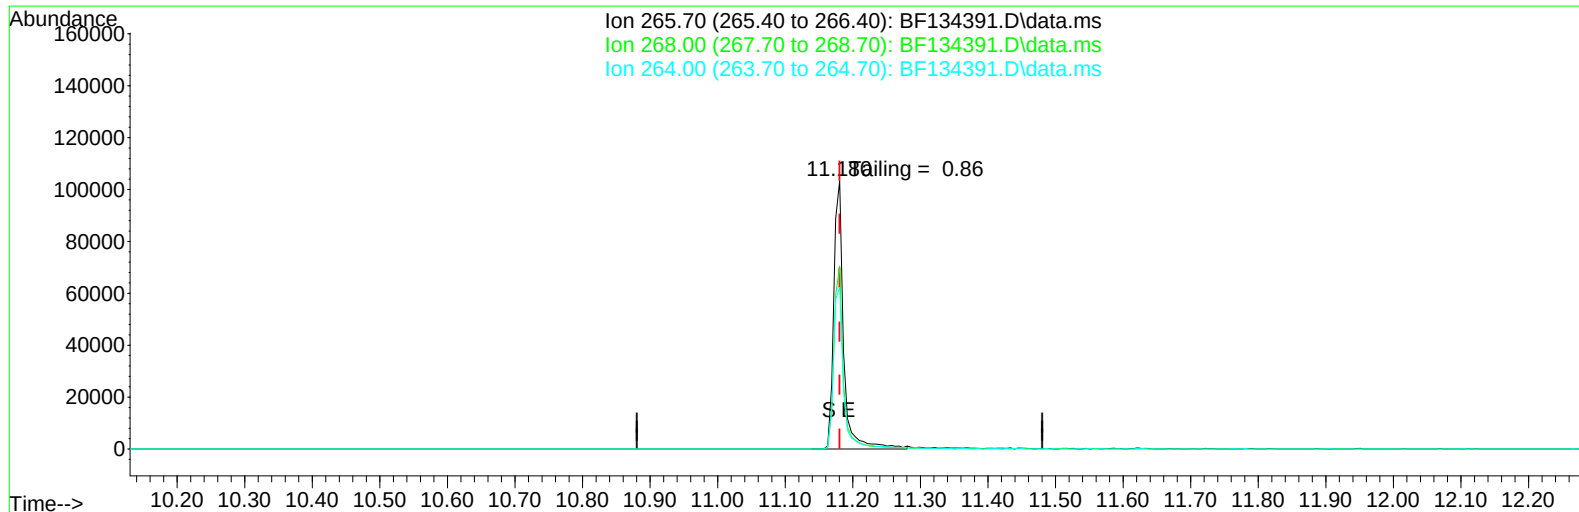

TIC: BF134391.D\data.ms

(70) Pentachlorophenol (C)

11.180min (+ 0.000) 29795.98 ng




response 105352

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	68.15
264.00	63.30	60.16
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072123\
 Data File : BF134391.D
 Acq On : 21 Jul 2023 09:26
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Quant Time: Jul 21 13:25:09 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Jul 14 22:51:27 2023
 Response via : Initial Calibration

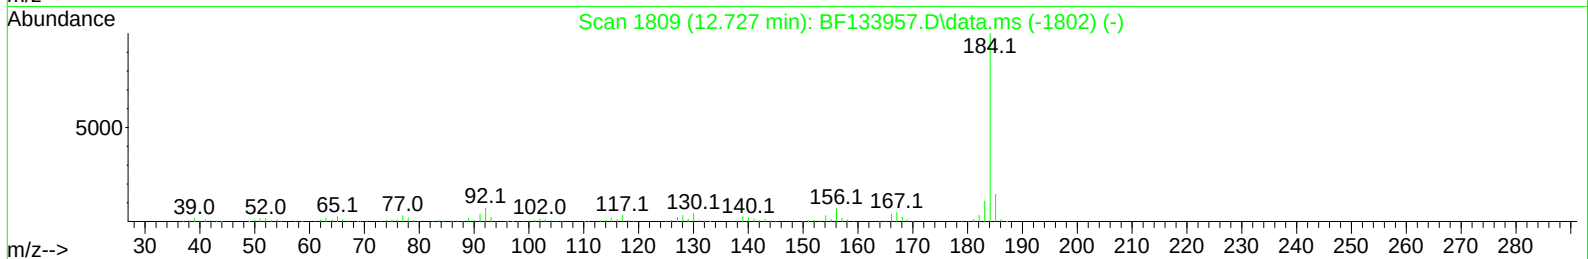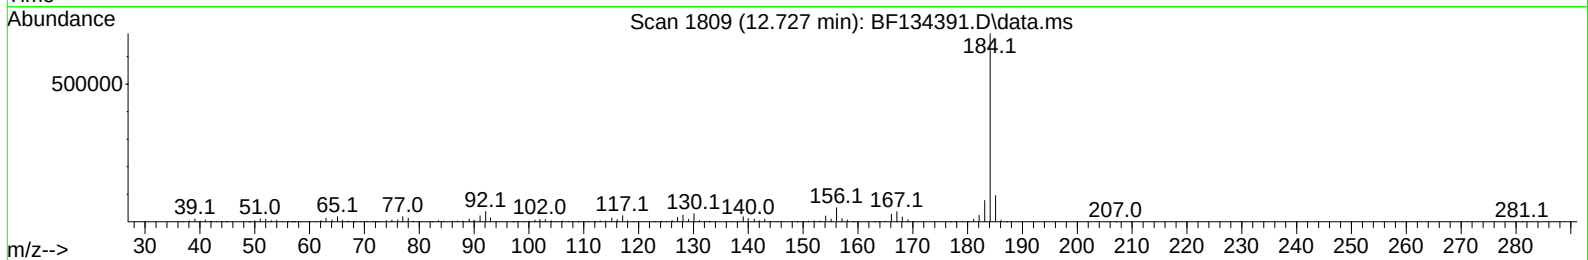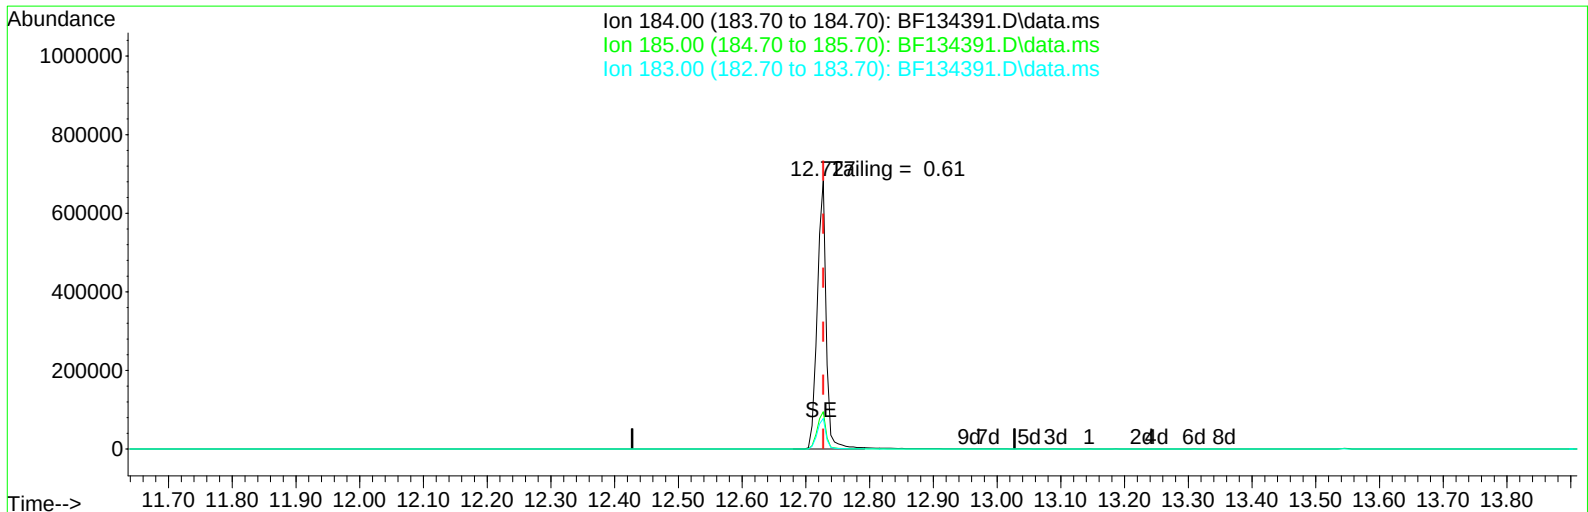

TIC: BF134391.D\data.ms

(77) Benzidine

12.727min (+ 0.000) 512030.47 ng m

response 657905

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.92
183.00	11.00	11.38
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/21/2023	BNA_F	<u>BF134391.D</u>
Compound Name	Response	Retention Time
DDT	318571	13.545
DDD	6222	13.268
DDE	621	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6843	325414	2.10

Instrument :
BNA_F
ClientSampleId :
DFTPP