
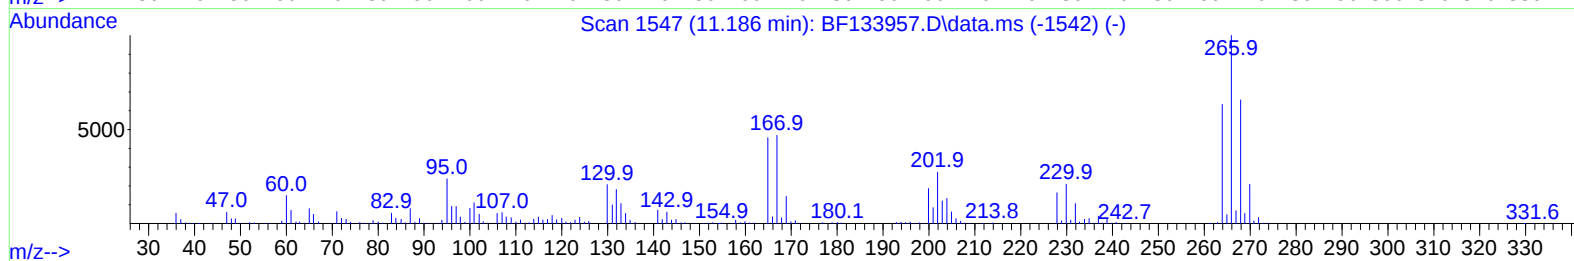
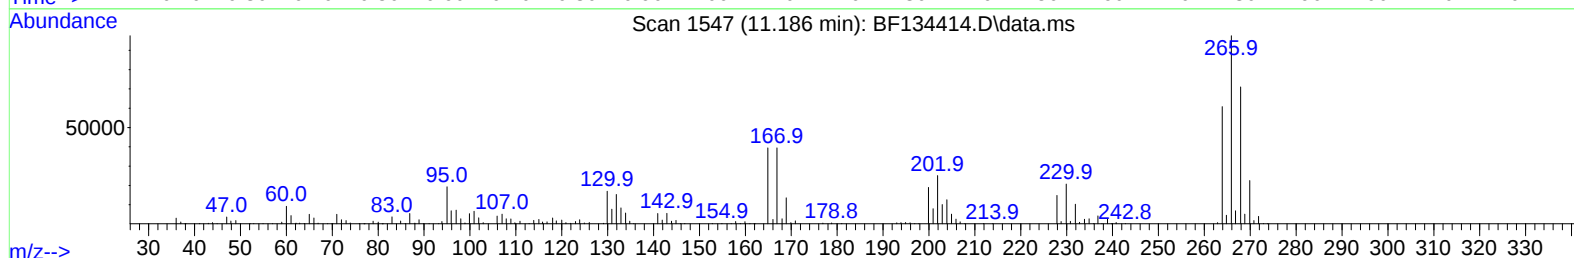


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072223\
Data File : BF134414.D
Acq On : 22 Jul 2023 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 14:11:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

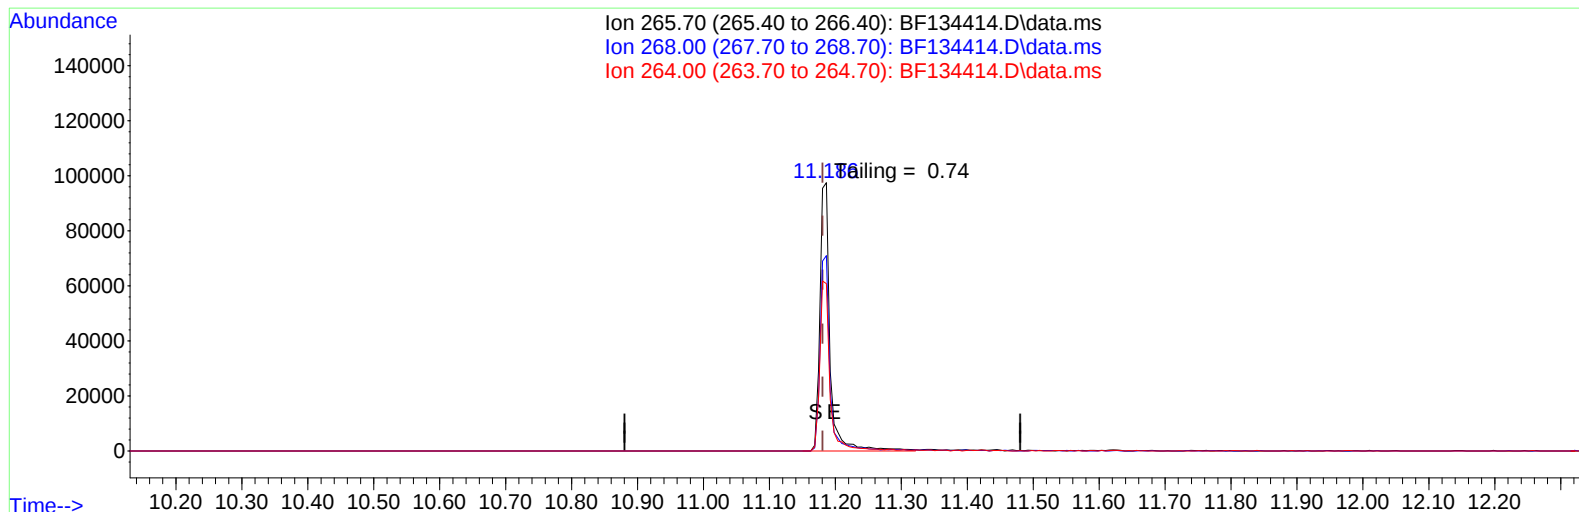

TIC: BF134414.D\data.ms

(70) Pentachlorophenol (C)




11.186min (+ 0.006) 34734.01 ng

response 104765

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	72.79
264.00	63.30	62.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072223\
Data File : BF134414.D
Acq On : 22 Jul 2023 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 22 14:11:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

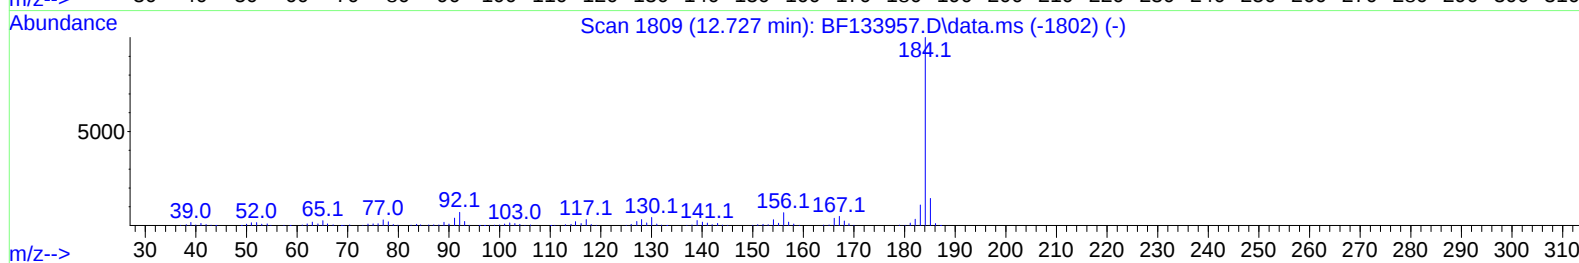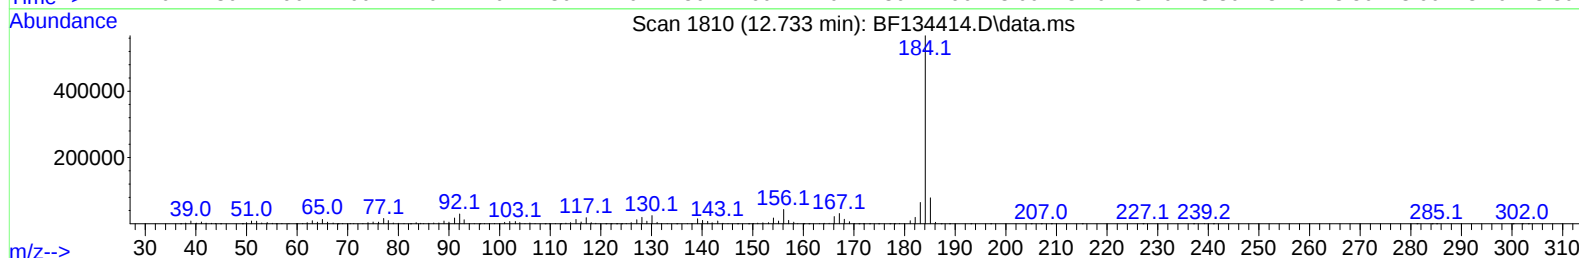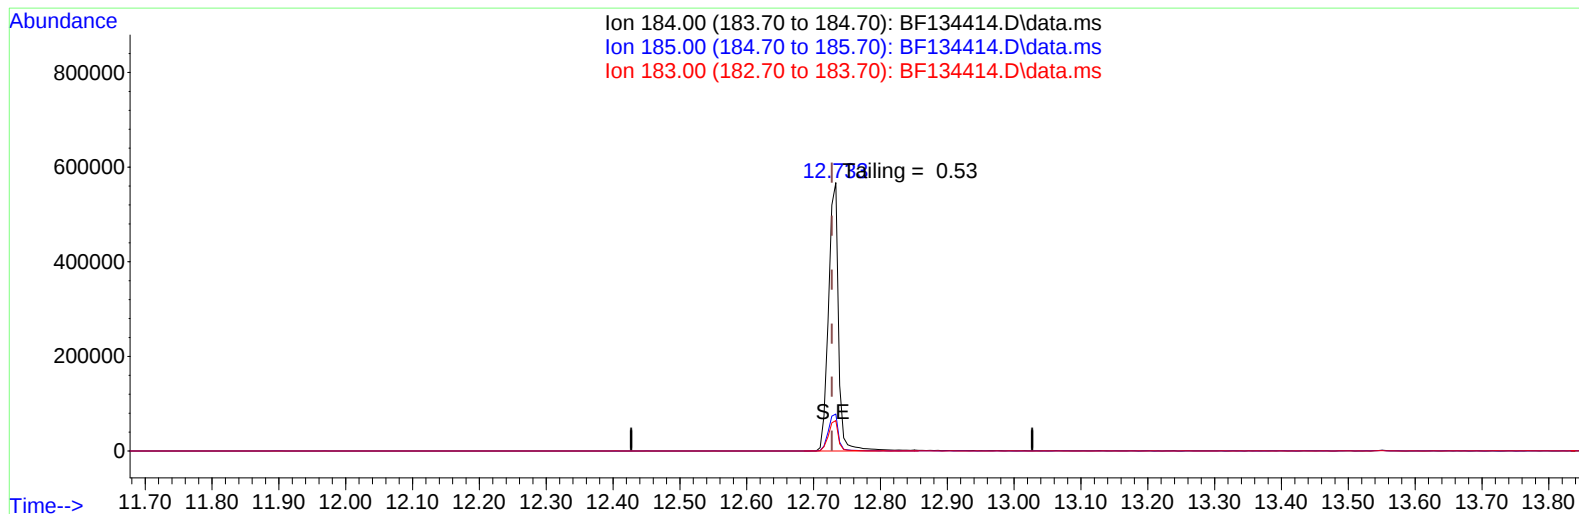

TIC: BF134414.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 116306.78 ng

response 581163

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.77
183.00	11.00	11.34
0.00	0.00	0.00