
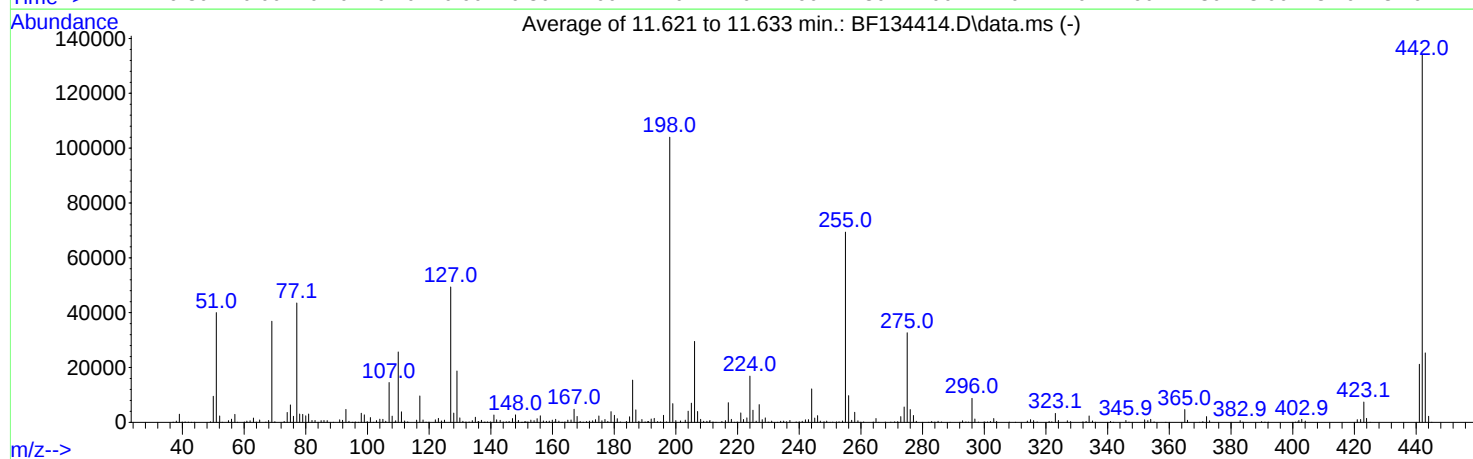


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072223\
 Data File : BF134414.D
 Acq On : 22 Jul 2023 10:05
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 14 22:51:27 2023

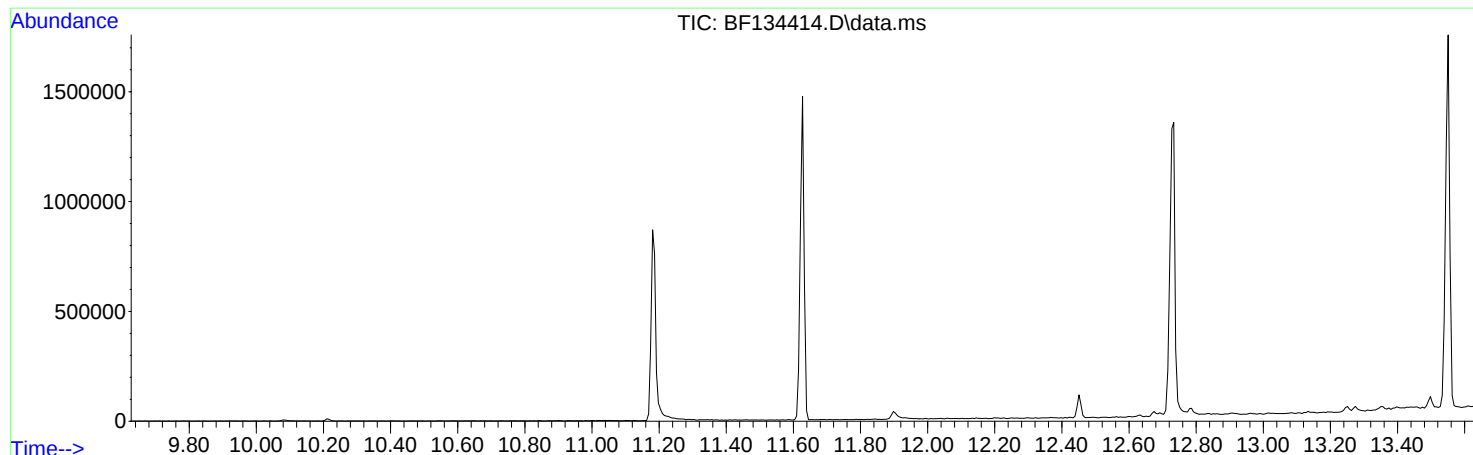

AutoFind: Scans 1621, 1622, 1623; Background Corrected with Scan 1616

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	38.5	40049	PASS
68	69	0.00	2	1.9	692	PASS
69	198	0.00	100	35.5	36906	PASS
70	69	0.00	2	0.7	244	PASS
127	198	10	80	47.5	49387	PASS
197	198	0.00	2	0.2	173	PASS
198	198	100	100	100.0	103995	PASS
199	198	5	9	6.6	6829	PASS
275	198	10	60	31.4	32648	PASS
365	198	1	100	4.5	4693	PASS
441	198	0.01	100	20.4	21190	PASS
442	442	50	100	100.0	134141	PASS
443	442	15	24	18.9	25323	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/22/2023	BNA_F	<u>BF134414.D</u>
Compound Name	Response	Retention Time
DDT	288191	13.551
DDD	8339	13.251
DDE	707	12.91
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
9046	297237	3.04

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072223\
Data File : BF134414.D
Acq On : 22 Jul 2023 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 14:11:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

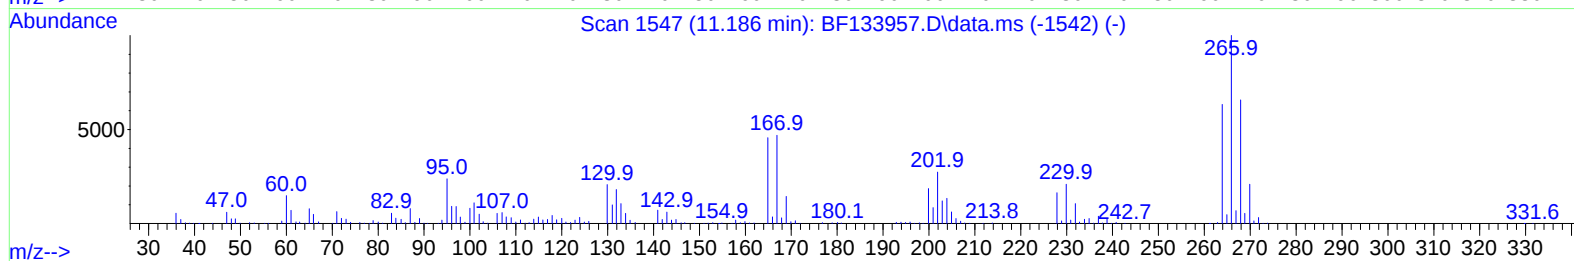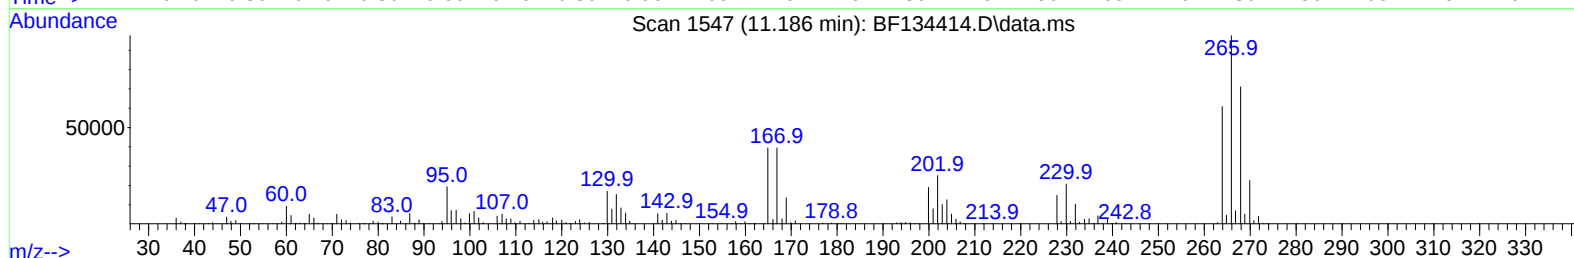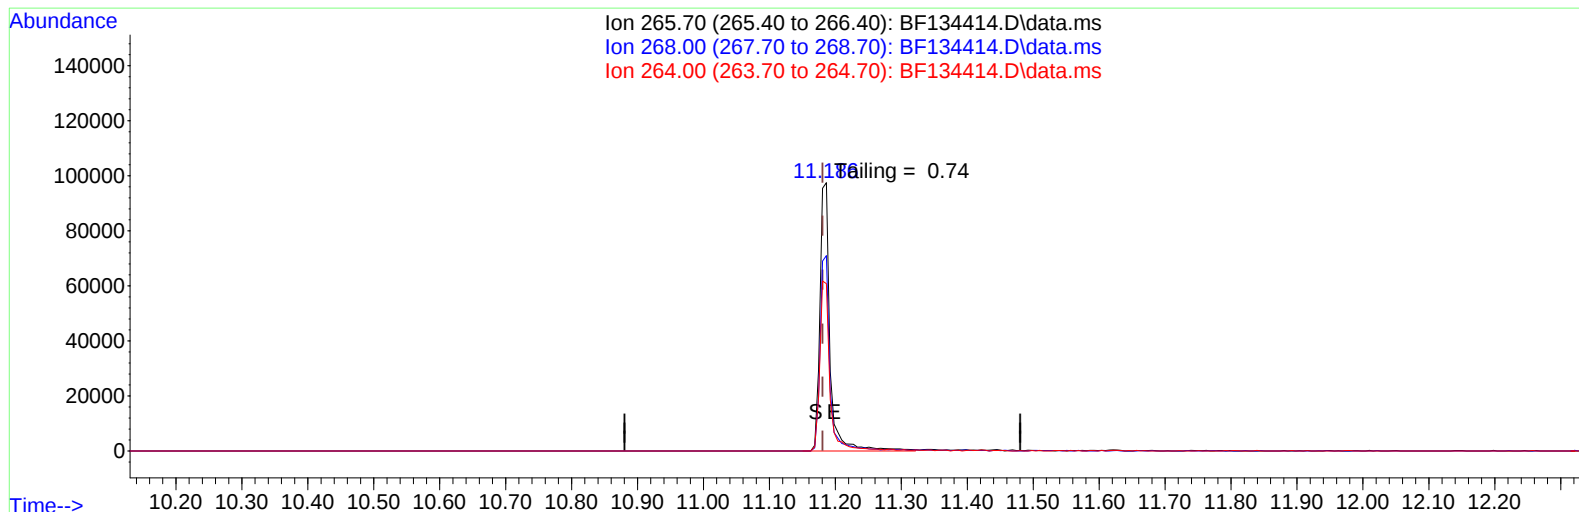

TIC: BF134414.D\data.ms

(70) Pentachlorophenol (C)

11.186min (+ 0.006) 34734.01 ng




response 104765

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	65.80	72.79
264.00	63.30	62.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072223\
Data File : BF134414.D
Acq On : 22 Jul 2023 10:05
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 22 14:11:30 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF062623.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 14 22:51:27 2023
Response via : Initial Calibration

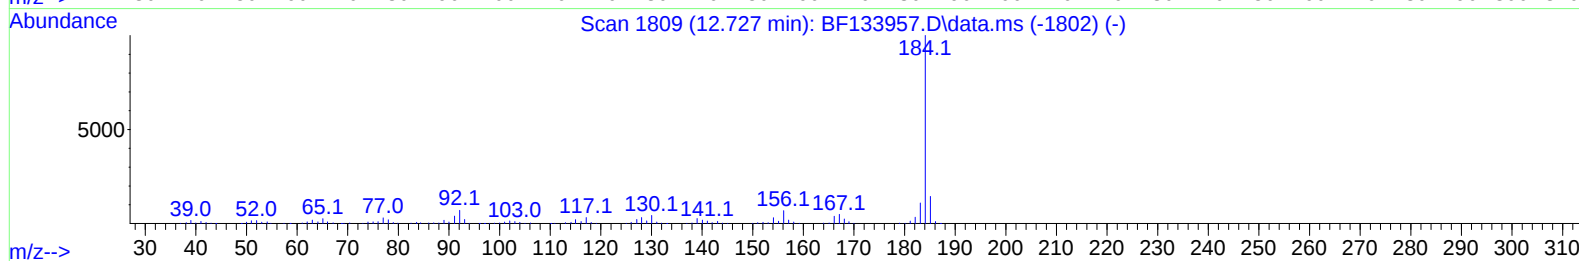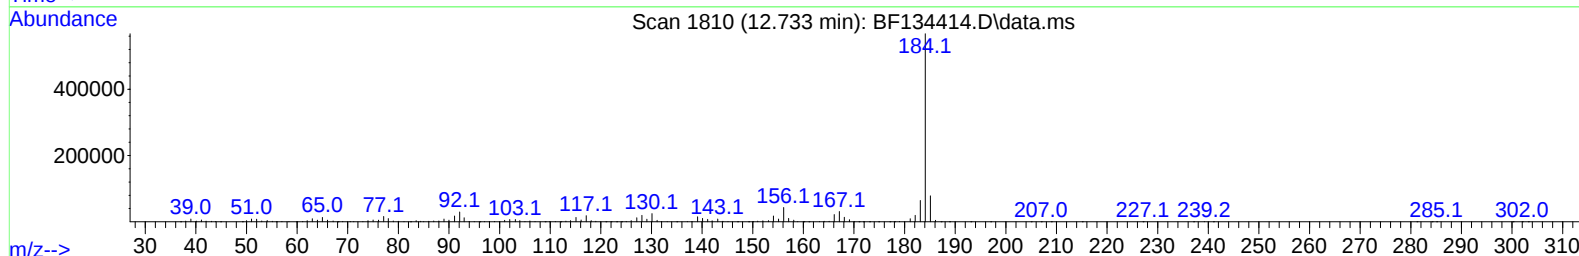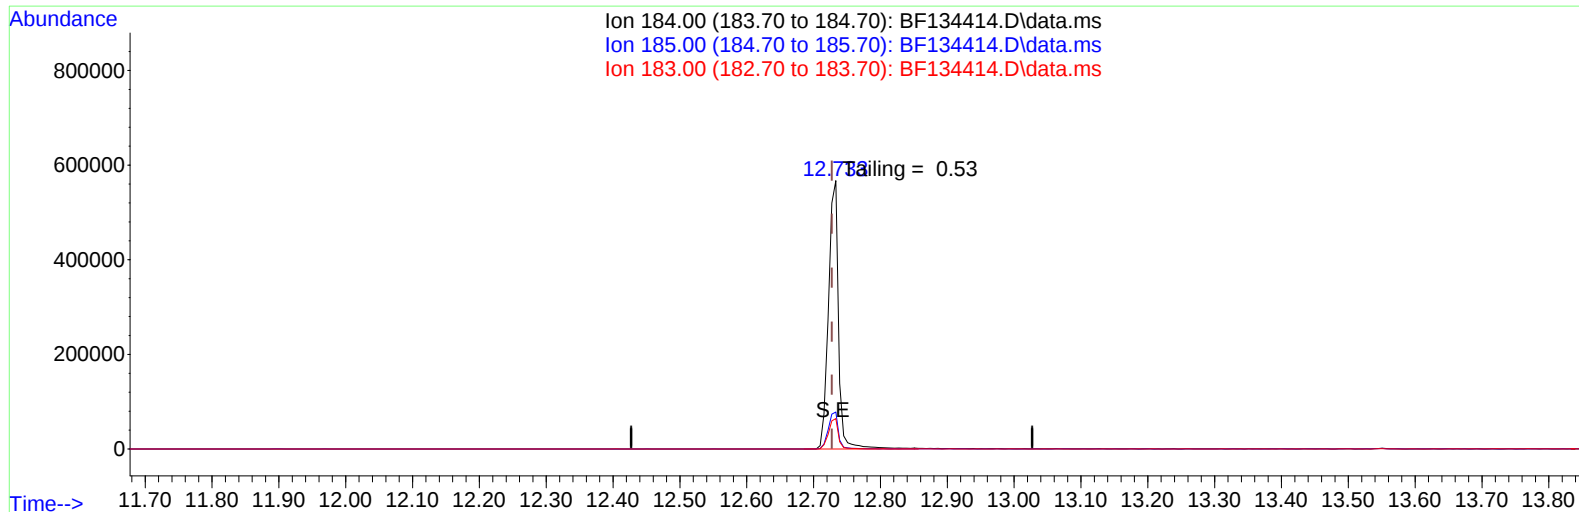

TIC: BF134414.D\data.ms

(77) Benzidine

12.733min (+ 0.006) 116306.78 ng

response 581163

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.50	13.77
183.00	11.00	11.34
0.00	0.00	0.00