


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072318\
 Data File : BF107579.D
 Acq On : 23 Jul 2018 10:45
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 16:29:27 2018

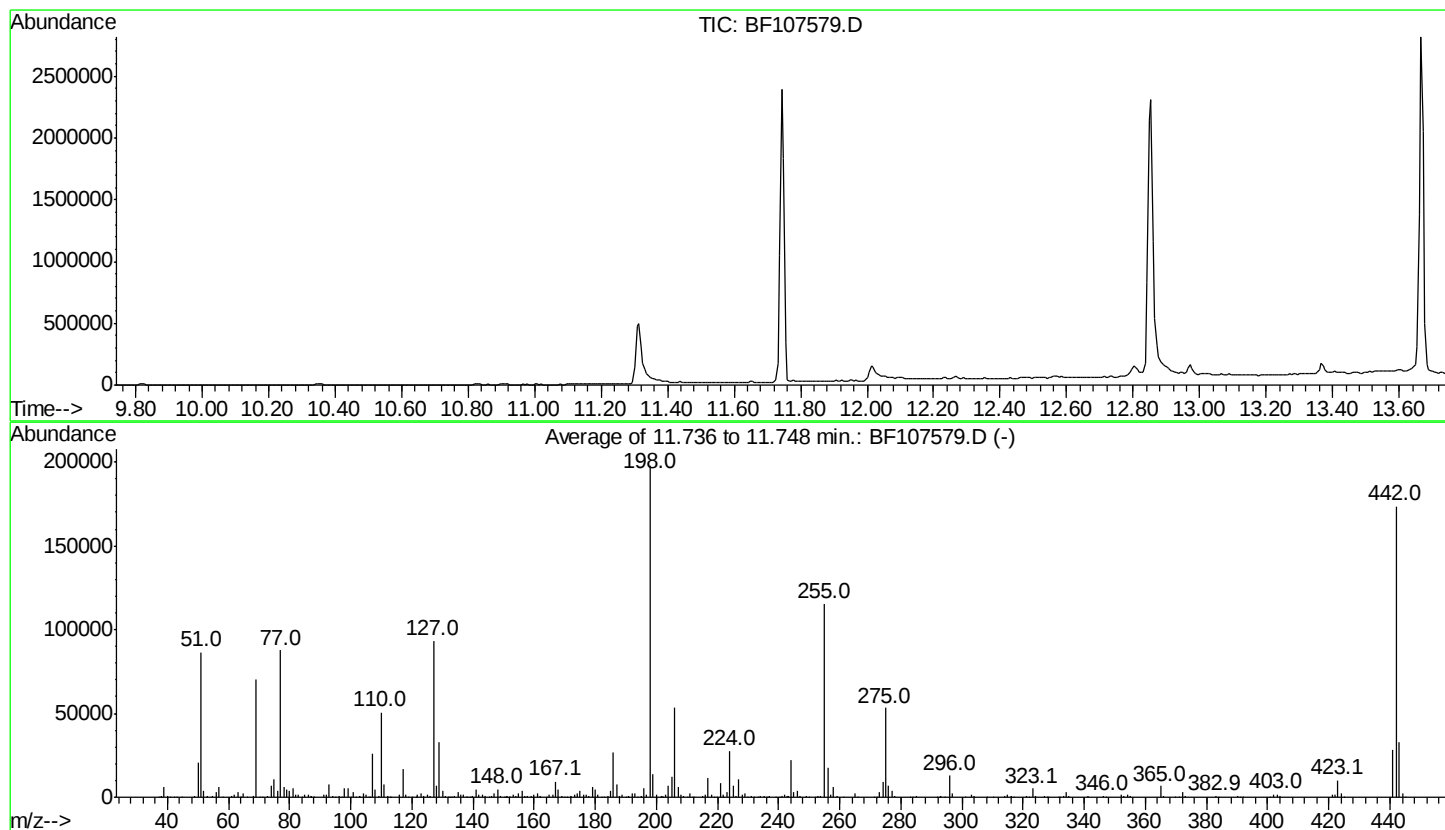

AutoFind: Scans 1598, 1599, 1600; Background Corrected with Scan 1593

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	43.8	86621	PASS
68	69	0.00	2	1.2	874	PASS
69	198	0.00	100	35.5	70206	PASS
70	69	0.00	2	0.4	298	PASS
127	198	10	80	47.2	93349	PASS
197	198	0.00	2	0.8	1660	PASS
198	198	100	100	100.0	197826	PASS
199	198	5	9	6.8	13447	PASS
275	198	10	60	27.0	53442	PASS
365	198	1	100	3.4	6639	PASS
441	198	0.01	100	14.4	28473	PASS
442	198	50	100	87.7	173528	PASS
443	442	15	24	18.8	32666	PASS