


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072318\
 Data File : BF107605.D
 Acq On : 23 Jul 2018 23:49
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 16:29:27 2018

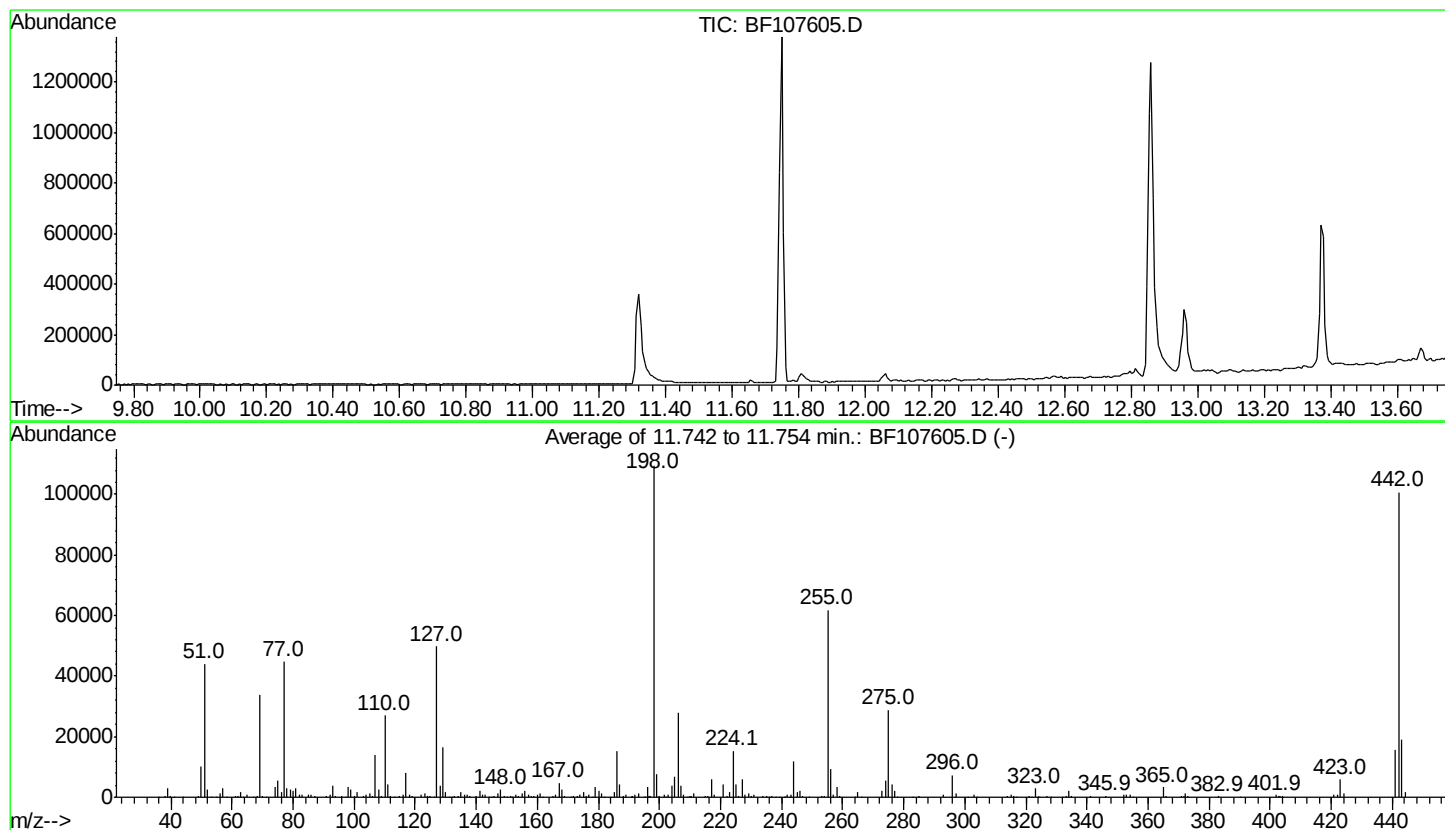

AutoFind: Scans 1599, 1600, 1601; Background Corrected with Scan 1594

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.2	44032	PASS
68	69	0.00	2	1.8	625	PASS
69	198	0.00	100	31.0	33985	PASS
70	69	0.00	2	1.6	545	PASS
127	198	10	80	45.5	49792	PASS
197	198	0.00	2	0.4	452	PASS
198	198	100	100	100.0	109506	PASS
199	198	5	9	6.8	7432	PASS
275	198	10	60	26.4	28944	PASS
365	198	1	100	3.0	3302	PASS
441	198	0.01	100	14.3	15694	PASS
442	198	50	100	91.9	100613	PASS
443	442	15	24	19.1	19206	PASS