

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072320\
 Data File : BF120989.D
 Acq On : 23 Jul 2020 19:23
 Operator : JU/CG
 Sample : PB130431BL
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB130431BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.434	563	569	572	rBV	3253377	3630946	74.78%	12.471%
2	6.445	735	741	744	rBV	3125646	3539260	72.89%	12.156%
3	6.810	799	803	807	rVB	1105216	854447	17.60%	2.935%
4	7.375	893	899	902	rBV	2446530	2435525	50.16%	8.365%
5	8.092	1017	1021	1025	rBV	1265149	1089283	22.43%	3.741%
6	9.169	1199	1204	1219	rBV	3899321	4573499	94.19%	15.708%
7	9.845	1314	1319	1336	rBV	1289353	1274630	26.25%	4.378%
8	10.633	1448	1453	1477	rBV	2544672	2996395	61.71%	10.291%
9	11.327	1567	1571	1579	rBV	1323010	1366531	28.14%	4.693%
10	12.921	1836	1842	1845	rBV	4306011	4855561	100.00%	16.677%
11	13.963	2015	2019	2034	rBV	1236727	1329314	27.38%	4.566%
12	15.410	2260	2265	2279	rBV	739327	1170081	24.10%	4.019%


Sum of corrected areas: 29115472

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072320\
Data File : BF120989.D
Acq On : 23 Jul 2020 19:23
Operator : JU/CG
Sample : PB130431BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130431BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

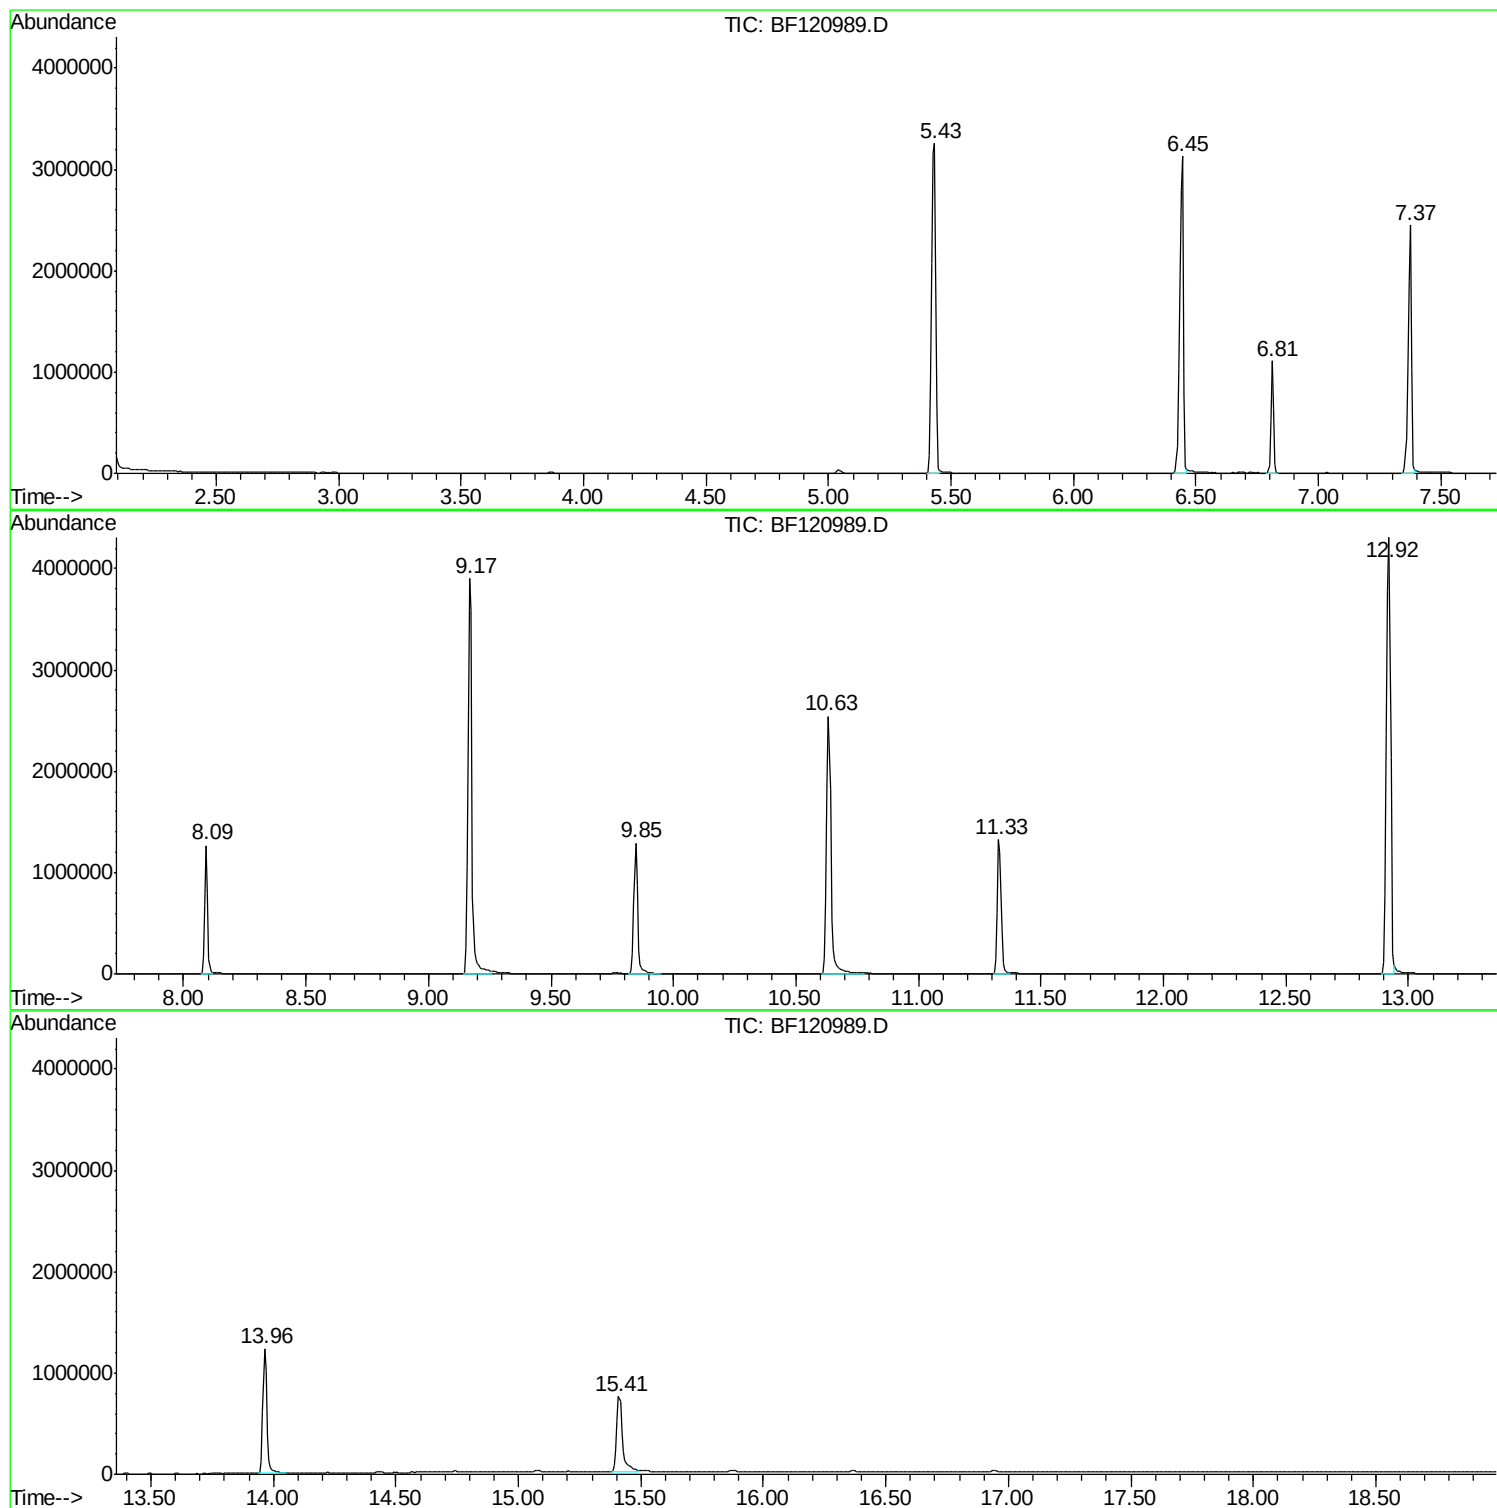

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072320\
Data File : BF120989.D
Acq On : 23 Jul 2020 19:23
Operator : JU/CG
Sample : PB130431BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130431BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072320\
Data File : BF120989.D
Acq On : 23 Jul 2020 19:23
Operator : JU/CG
Sample : PB130431BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB130431BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071620.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc