
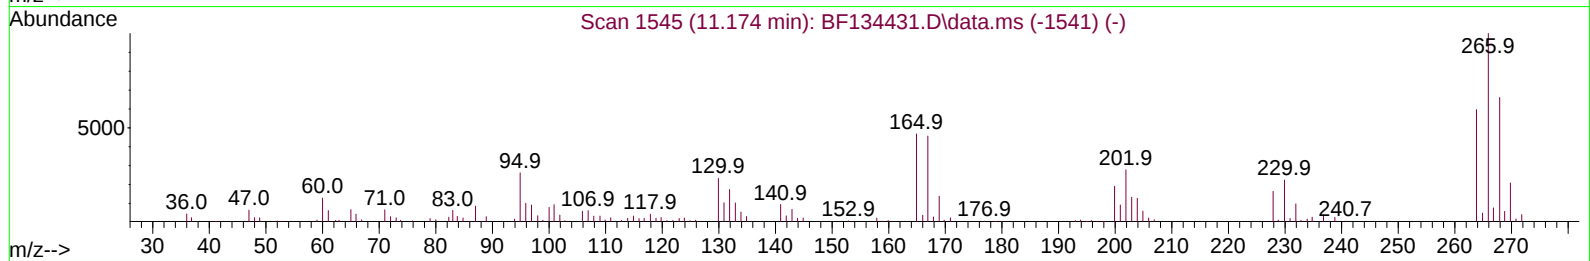
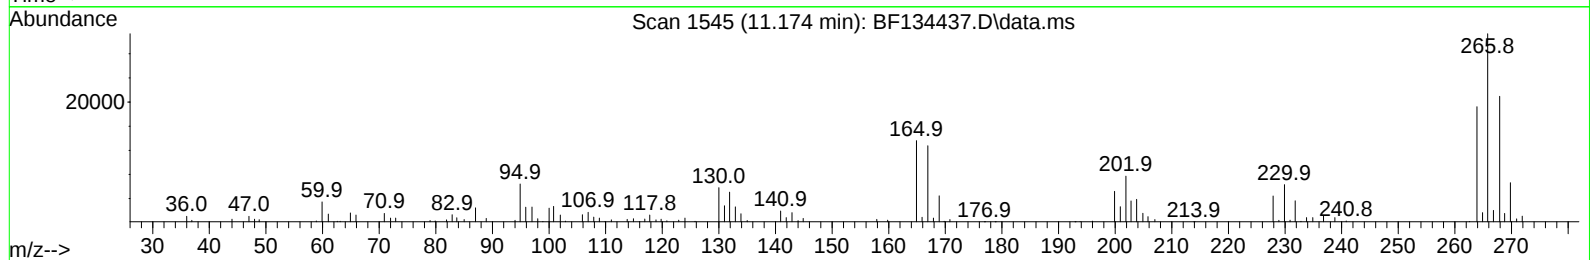


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072423\
Data File : BF134437.D
Acq On : 24 Jul 2023 19:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 05:32:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

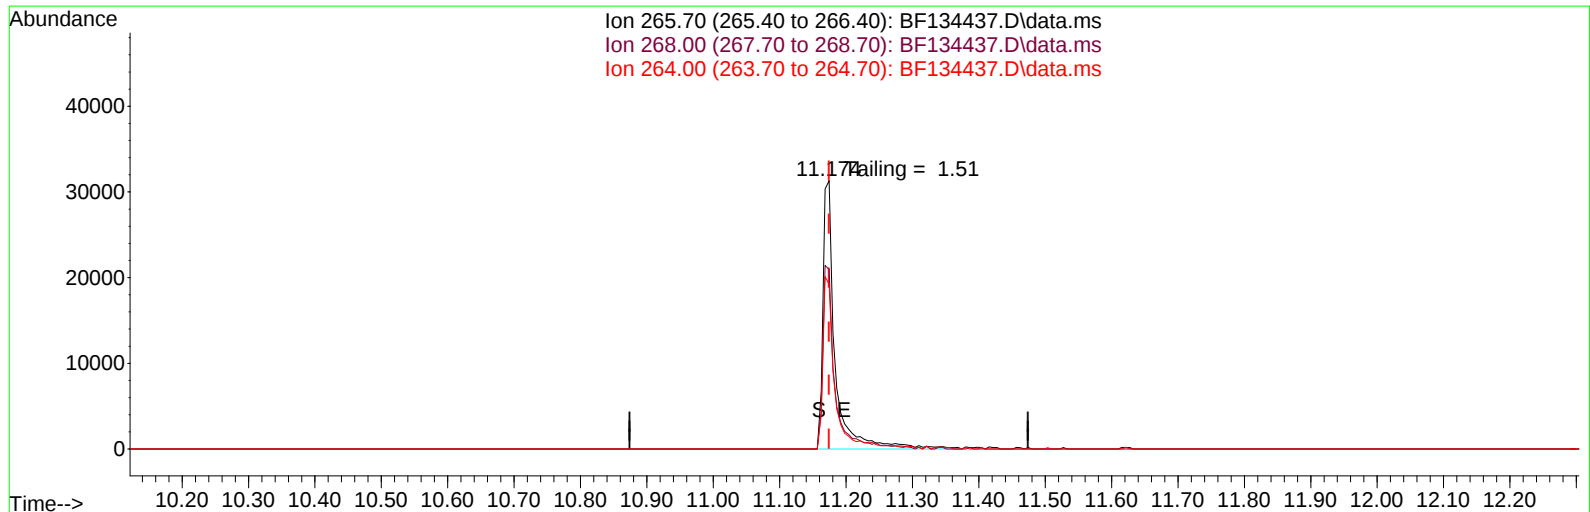

TIC: BF134437.D\data.ms

(70) Pentachlorophenol (C)




11.174min (+ 0.000) 43960.98 ng

response 39606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	66.87
264.00	59.70	61.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072423\
Data File : BF134437.D
Acq On : 24 Jul 2023 19:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 05:32:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

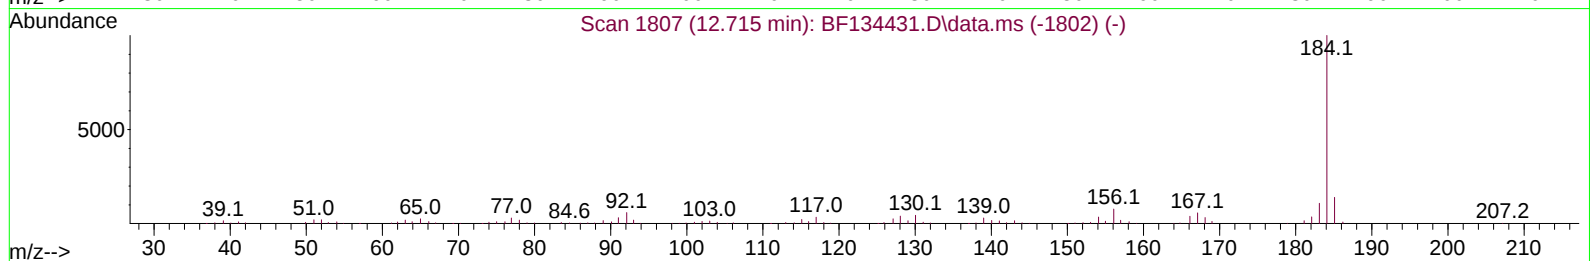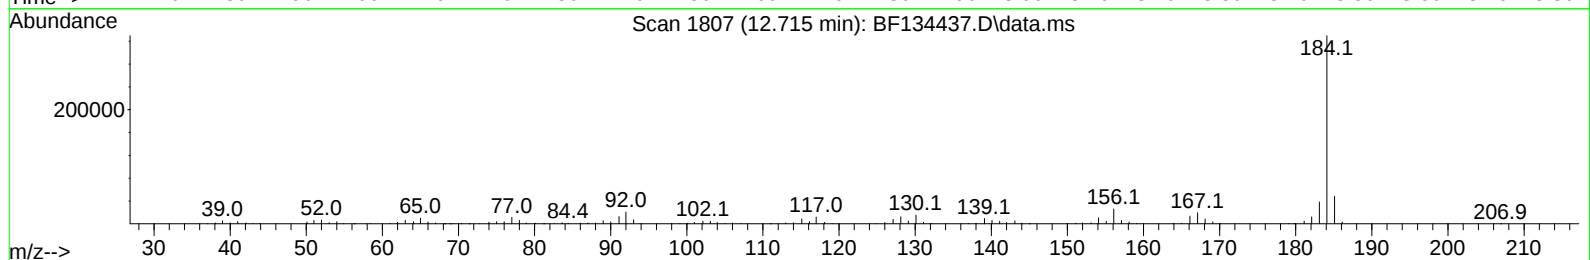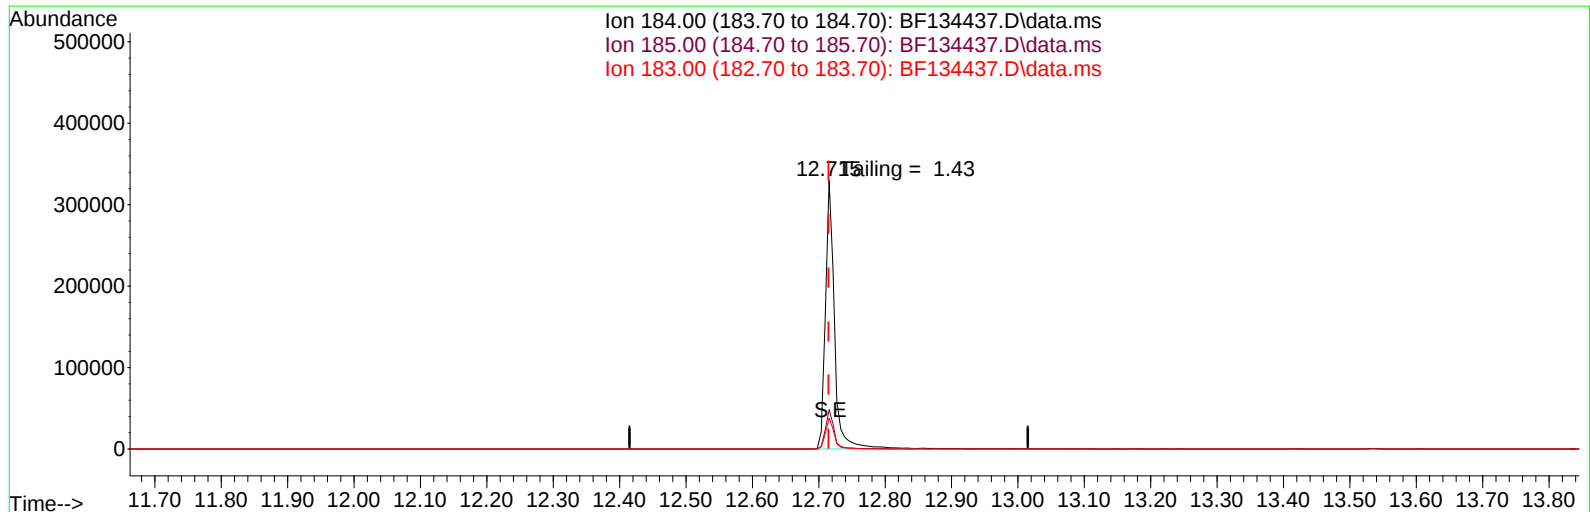

TIC: BF134437.D\data.ms

(77) Benzidine

12.715min (+ 0.000) 0.00 ng

response 313379

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.71
183.00	10.80	11.58
0.00	0.00	0.00