


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072423\
Data File : BF134437.D
Acq On : 24 Jul 2023 19:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 25 01:46:04 2023

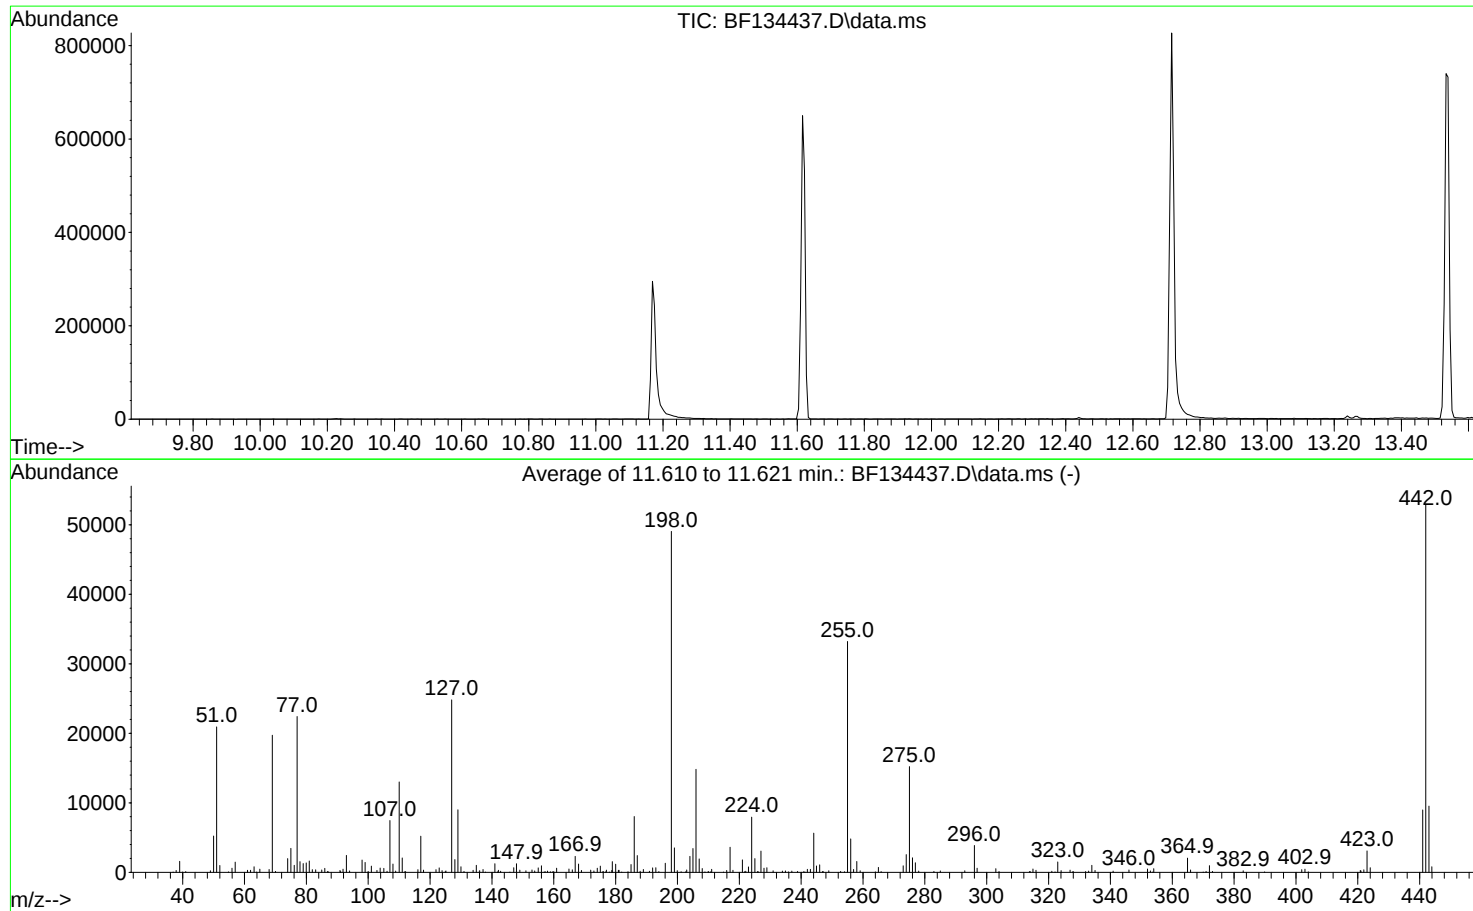

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1615

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.7	20925	PASS
68	69	0.00	2	2.1	406	FAIL*
69	198	0.00	100	40.2	19735	PASS
70	69	0.00	2	0.8	149	PASS
127	198	10	80	50.6	24805	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	49045	PASS
199	198	5	9	7.2	3520	PASS
275	198	10	60	31.0	15224	PASS
365	198	1	100	4.2	2055	PASS
441	198	0.01	100	18.3	8988	PASS
442	442	50	100	100.0	52919	PASS
443	442	15	24	18.0	9528	PASS

DDT Breakdown


Date	Instrument Name	DFTPP Data File
7/24/2023	BNA_F	<u>BF134437.D</u>
Compound Name	Response	Retention Time
DDT	136314	13.539
DDD	2907	13.268
DDE	127	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3034	139348	2.18

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072423\
Data File : BF134437.D
Acq On : 24 Jul 2023 19:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 05:32:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

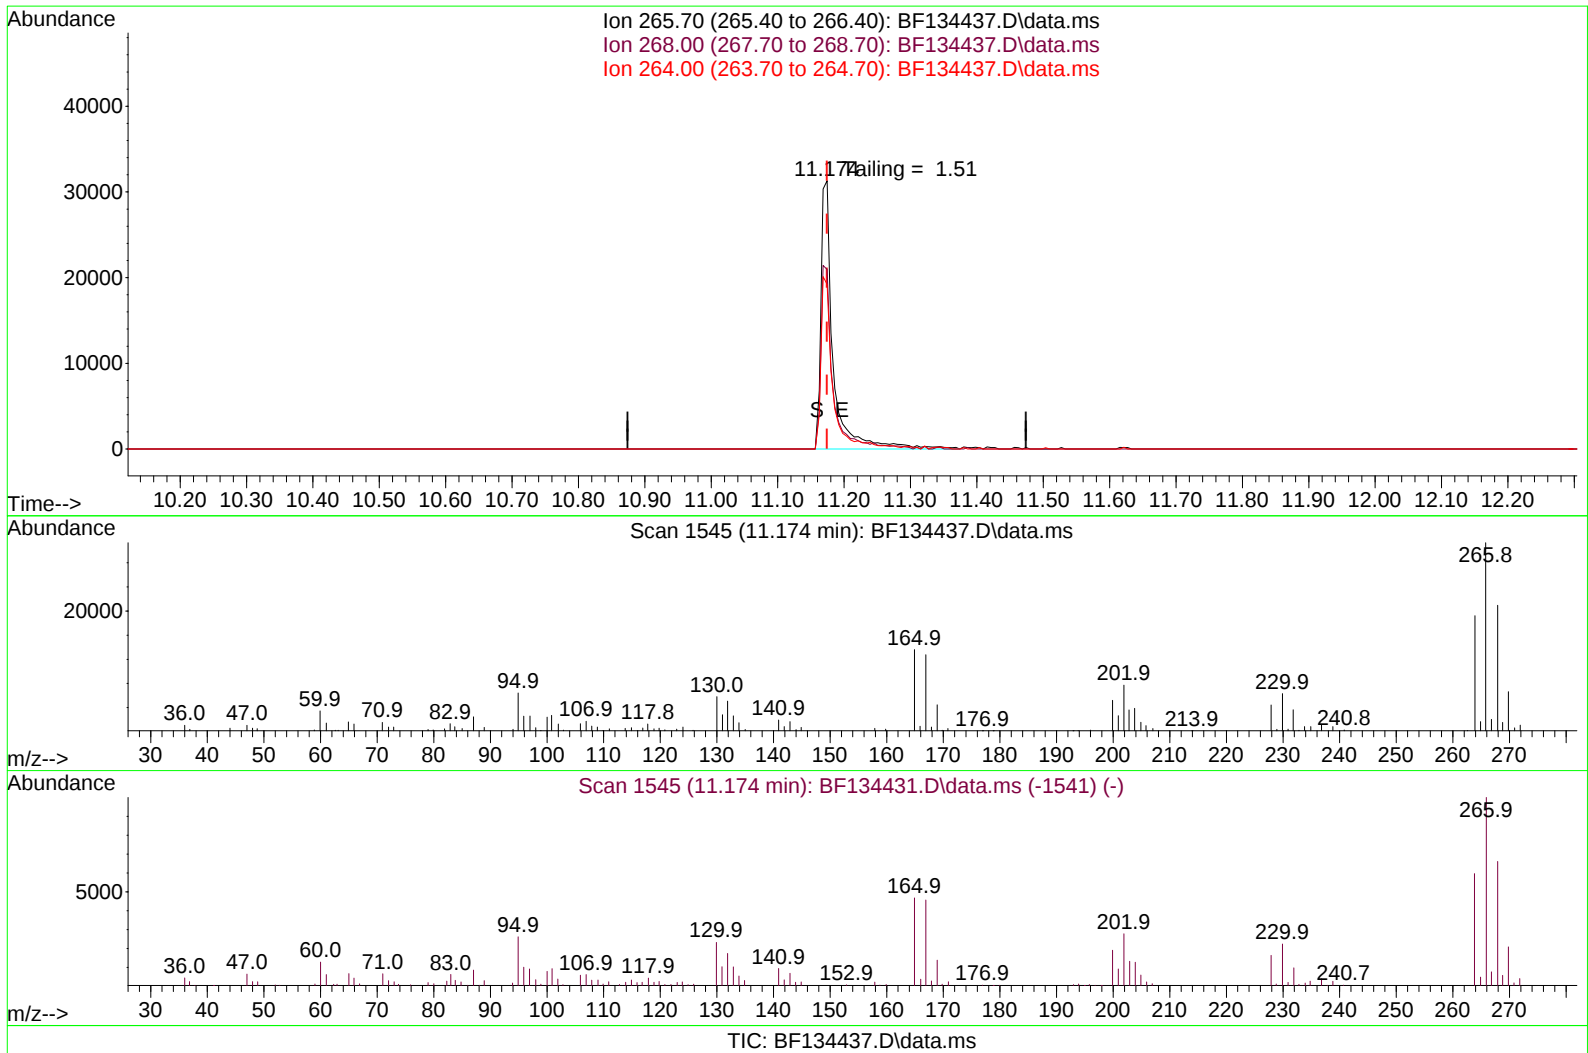

(70) Pentachlorophenol (C)

11.174min (+ 0.000) 43960.98 ng




response 39606

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	66.87
264.00	59.70	61.38
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072423\
Data File : BF134437.D
Acq On : 24 Jul 2023 19:22
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 25 05:32:53 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

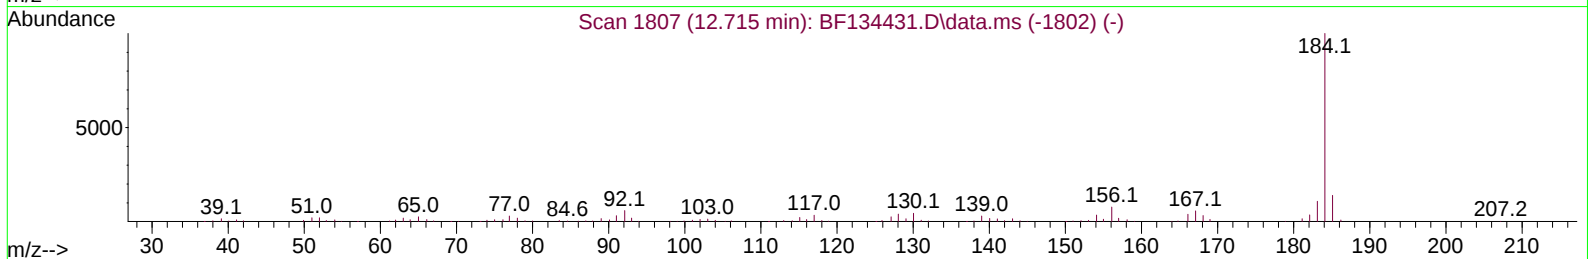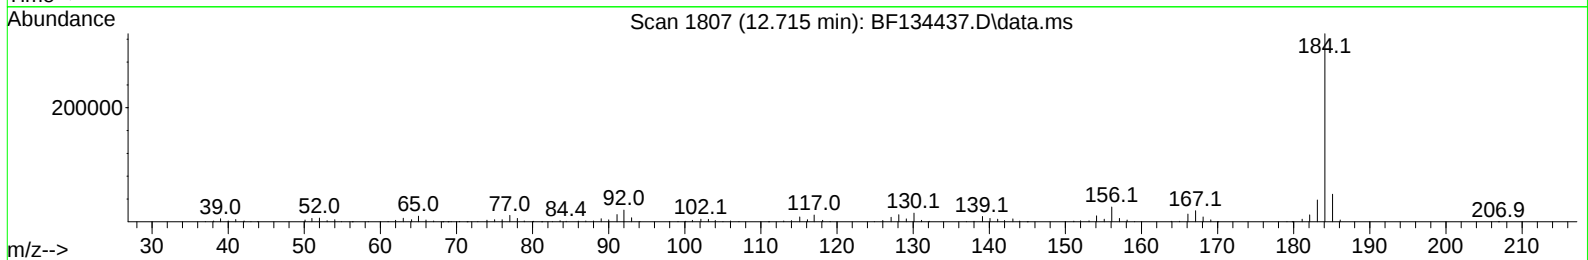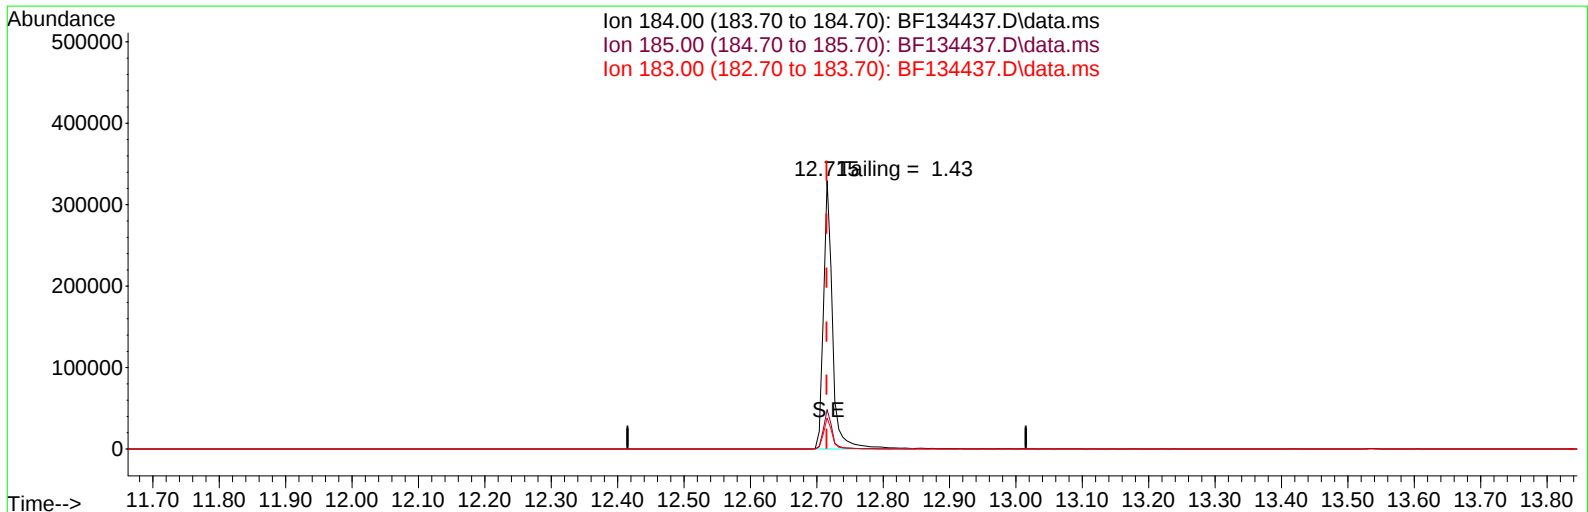

TIC: BF134437.D\data.ms

(77) Benzidine

12.715min (+ 0.000) 0.00 ng

response 313379

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	14.71
183.00	10.80	11.58
0.00	0.00	0.00