
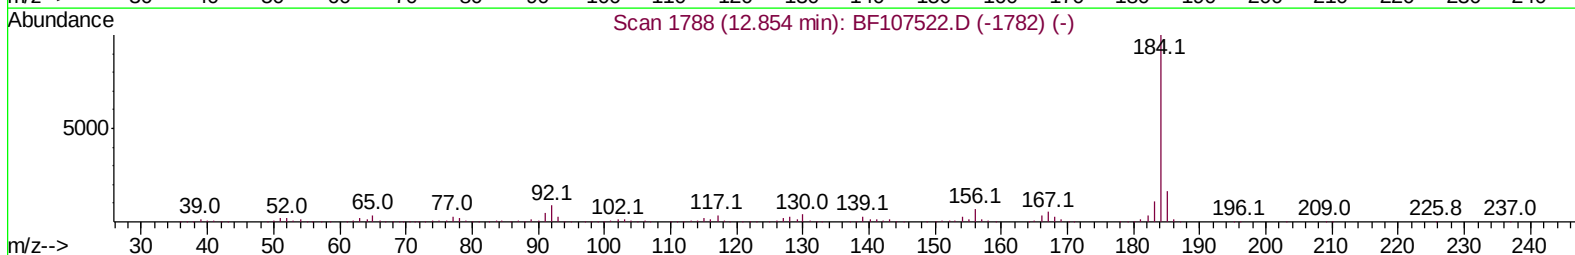
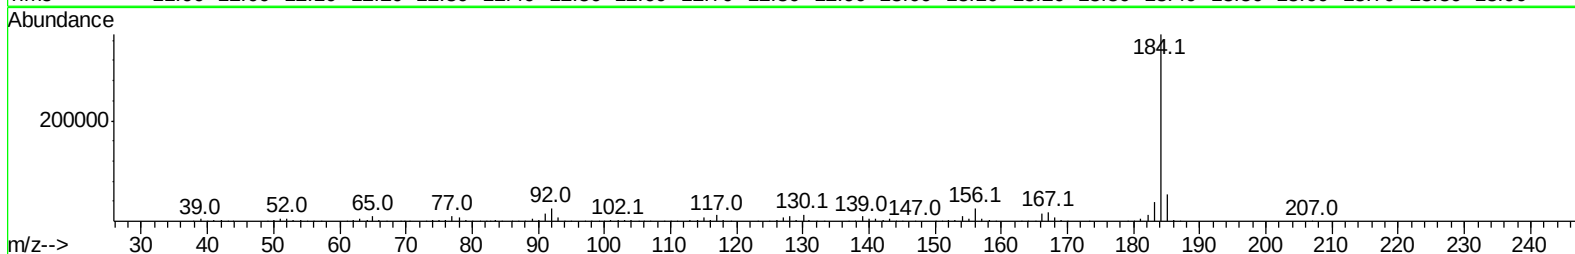


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072518\
Data File : BF107675.D
Acq On : 25 Jul 2018 23:53
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 08:29:35 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Jul 20 16:29:27 2018
Response via : Initial Calibration

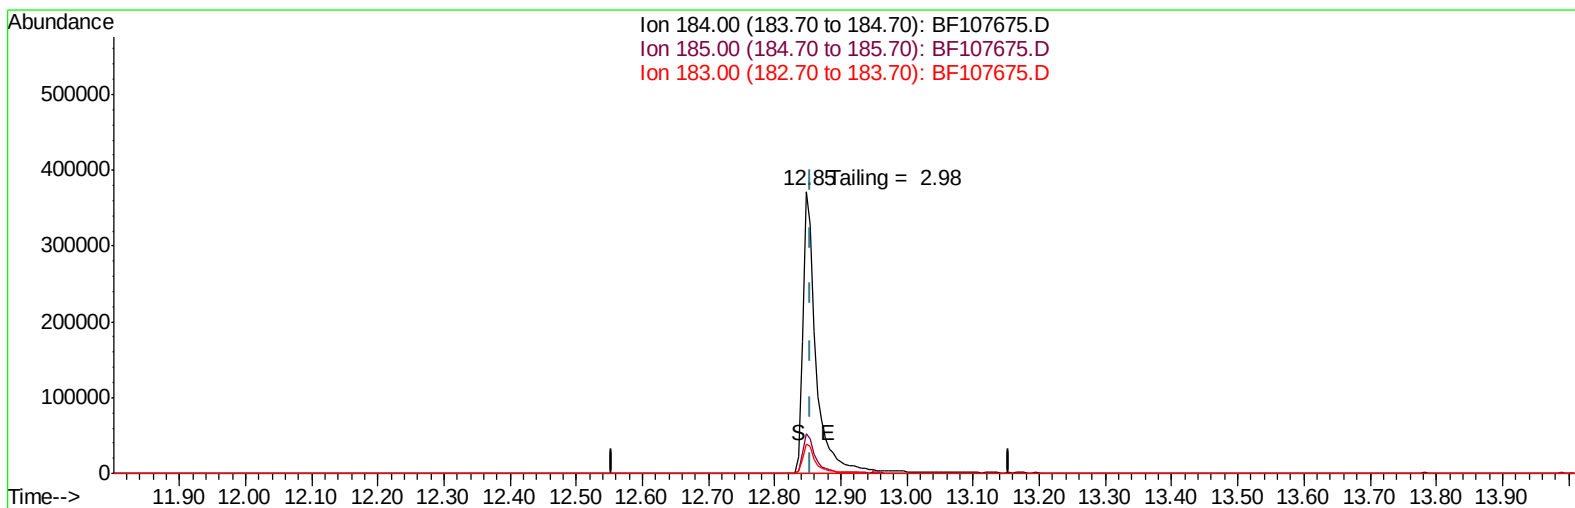

TIC: BF107675.D

(76) Benzidine

12.848min (-0.006) 156295.51ng

response 526621

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.16
183.00	11.60	10.68
0.00	0.00	0.00