
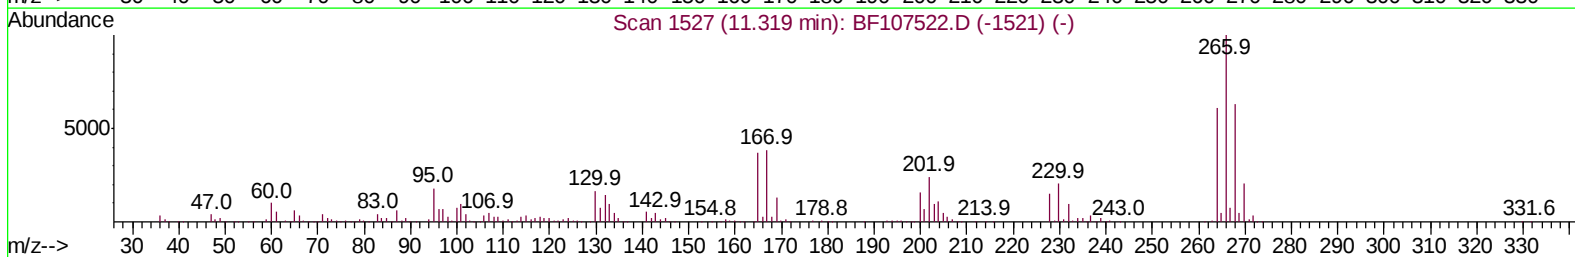
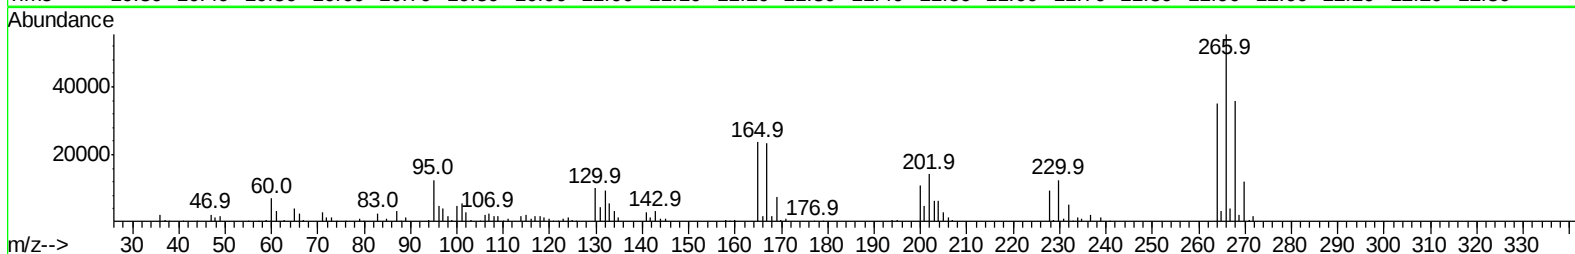


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072518\  
Data File : BF107675.D  
Acq On : 25 Jul 2018 23:53  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 08:29:35 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 20 16:29:27 2018  
Response via : Initial Calibration

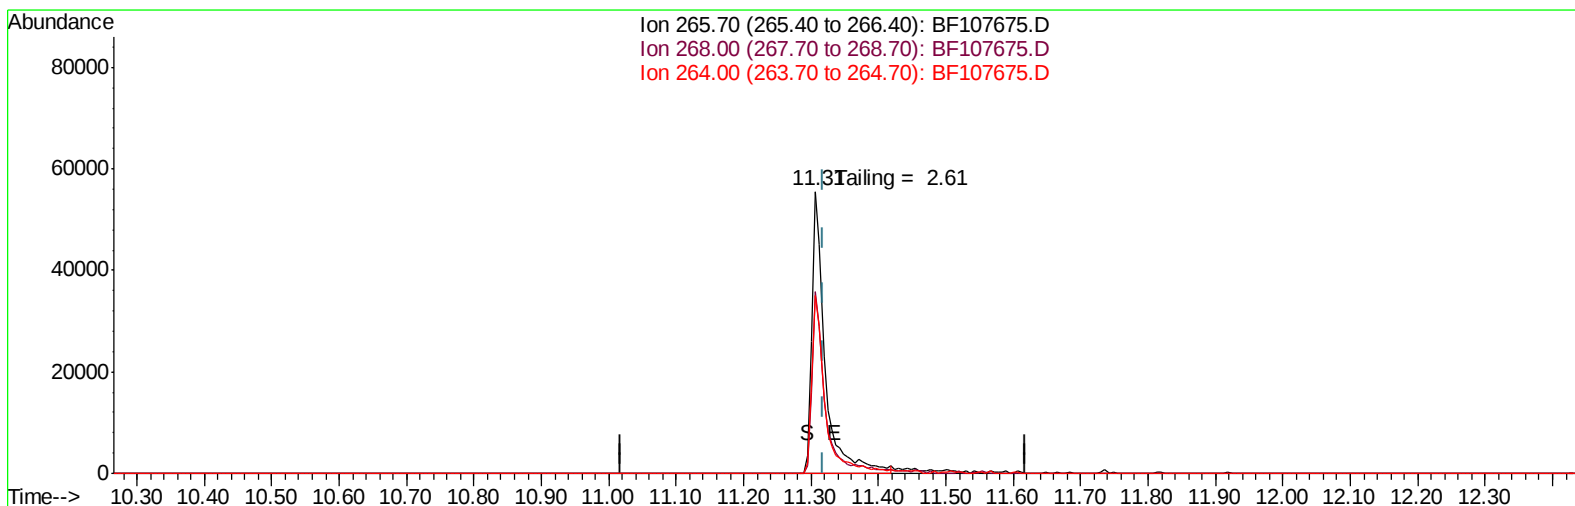

TIC: BF107675.D

(69) Pentachlorophenol (C)




11.307min (-0.012) 16100.83ng

response 75421

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 265.70 | 100   | 100   |
| 268.00 | 63.90 | 64.58 |
| 264.00 | 61.90 | 63.16 |
| 0.00   | 0.00  | 0.00  |

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072518\  
Data File : BF107675.D  
Acq On : 25 Jul 2018 23:53  
Operator : JU/SJ  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 08:29:35 2018  
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF072018.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Fri Jul 20 16:29:27 2018  
Response via : Initial Calibration

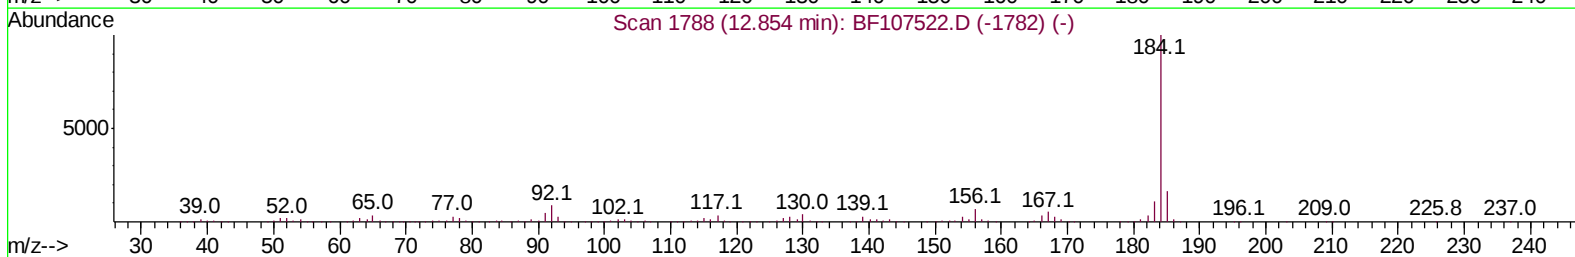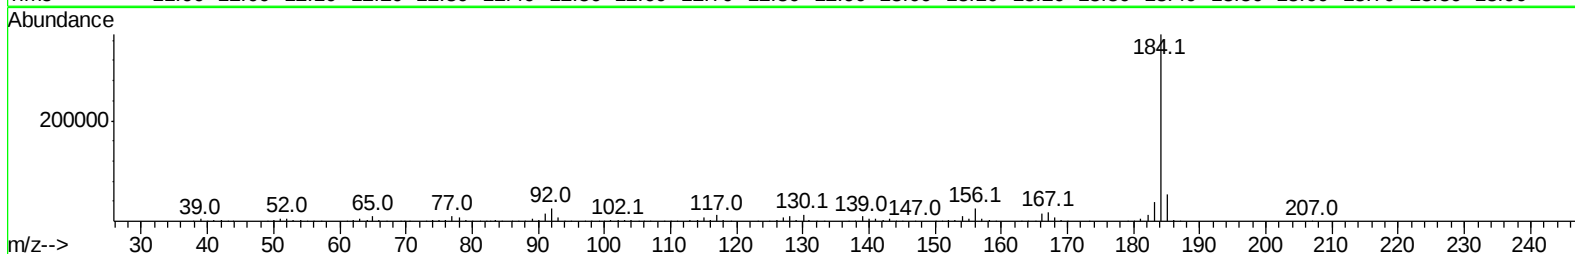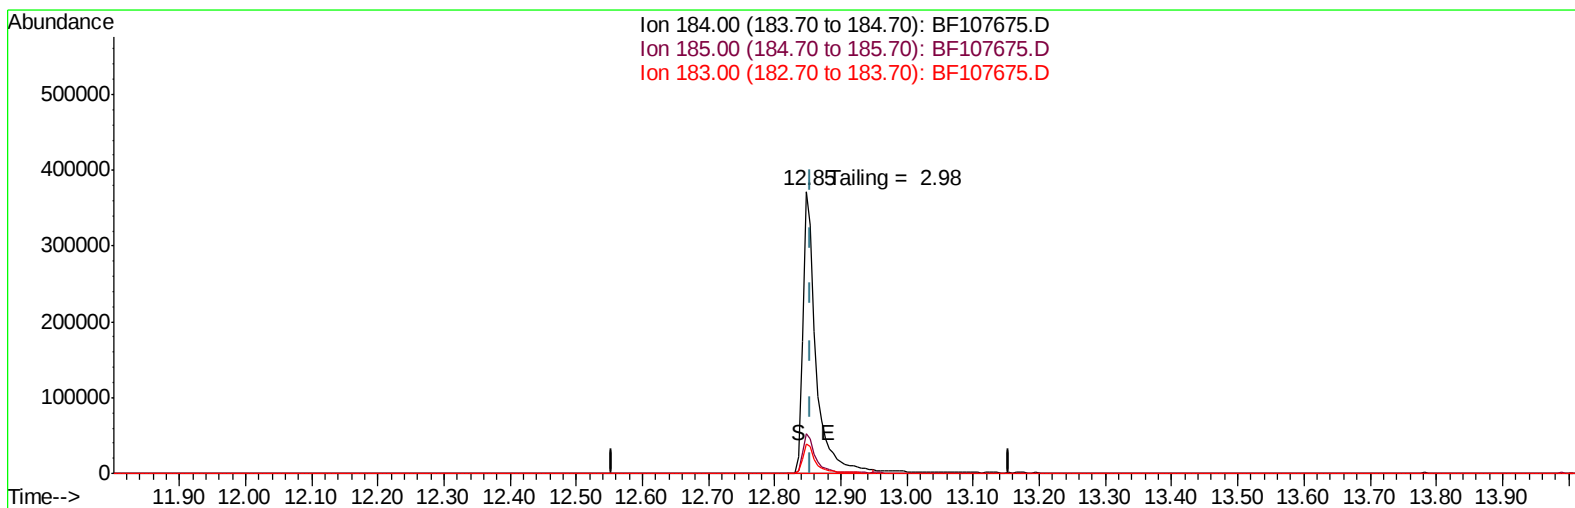

TIC: BF107675.D

(76) Benzidine

12.848min (-0.006) 156295.51ng

response 526621

| Ion    | Exp%  | Act%  |
|--------|-------|-------|
| 184.00 | 100   | 100   |
| 185.00 | 15.70 | 14.16 |
| 183.00 | 11.60 | 10.68 |
| 0.00   | 0.00  | 0.00  |