


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072518\
 Data File : BF107648.D
 Acq On : 25 Jul 2018 11:13
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 16:29:27 2018

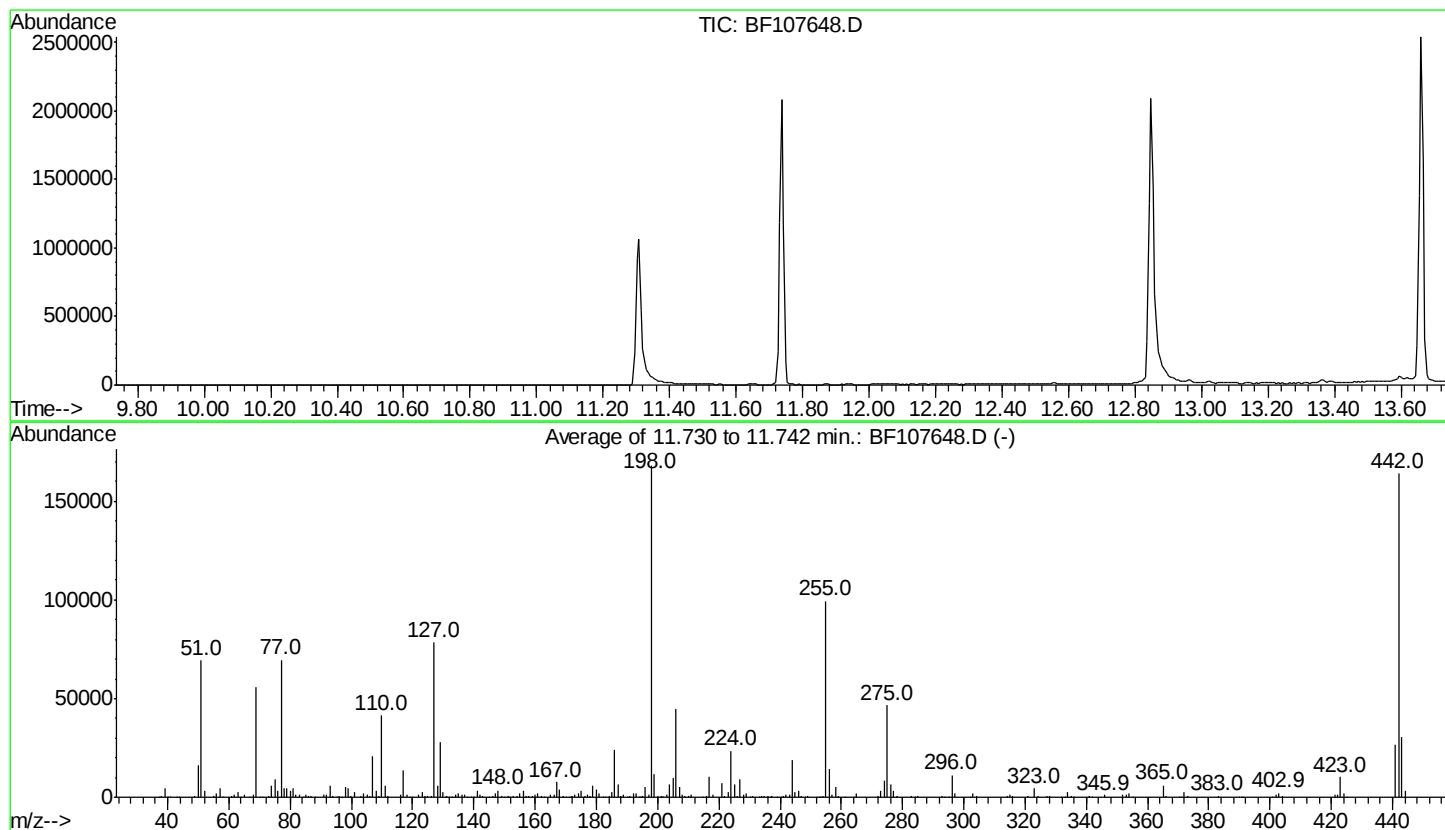

AutoFind: Scans 1597, 1598, 1599; Background Corrected with Scan 1592

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.2	69202	PASS
68	69	0.00	2	1.9	1058	PASS
69	198	0.00	100	33.4	56116	PASS
70	69	0.00	2	0.5	285	PASS
127	198	10	80	46.6	78250	PASS
197	198	0.00	2	0.8	1414	PASS
198	198	100	100	100.0	168072	PASS
199	198	5	9	6.8	11497	PASS
275	198	10	60	27.8	46677	PASS
365	198	1	100	3.6	6076	PASS
441	198	0.01	100	15.7	26318	PASS
442	198	50	100	97.6	164101	PASS
443	442	15	24	18.5	30322	PASS