
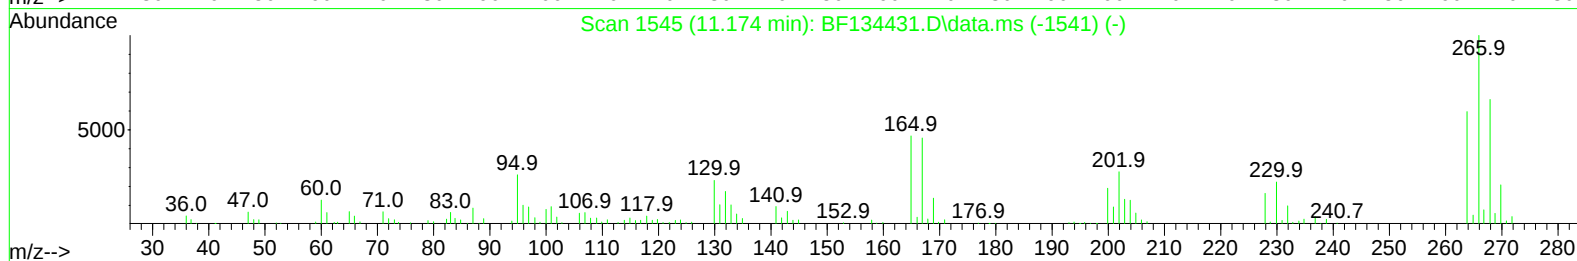
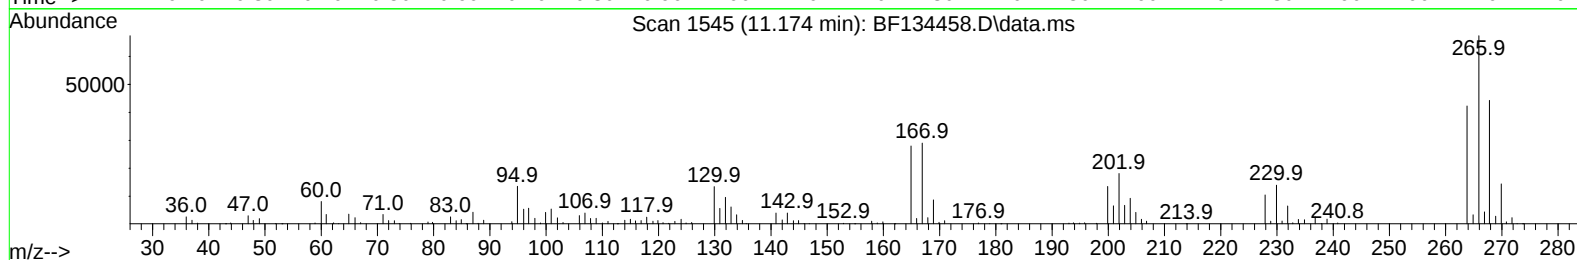


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072523\
Data File : BF134458.D
Acq On : 25 Jul 2023 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 14:20:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

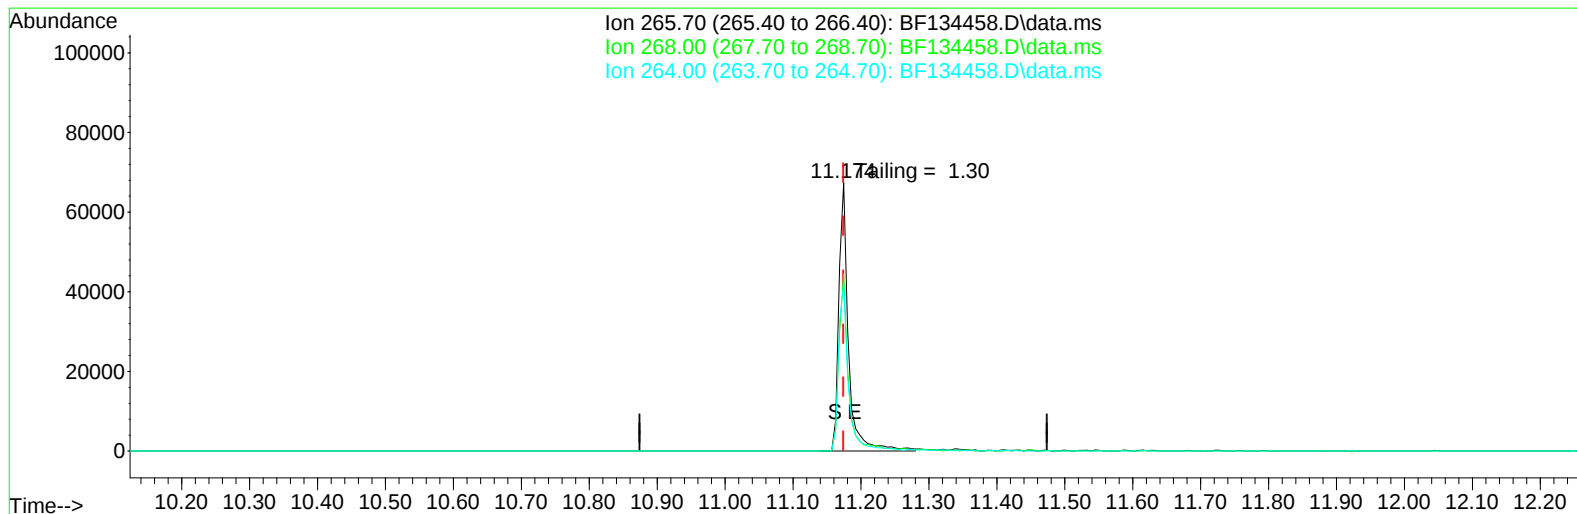

TIC: BF134458.D\data.ms

(70) Pentachlorophenol (C)




11.174min (+ 0.000) 29454.52 ng

response 65579

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	65.74
264.00	59.70	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072523\
Data File : BF134458.D
Acq On : 25 Jul 2023 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 25 14:20:17 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

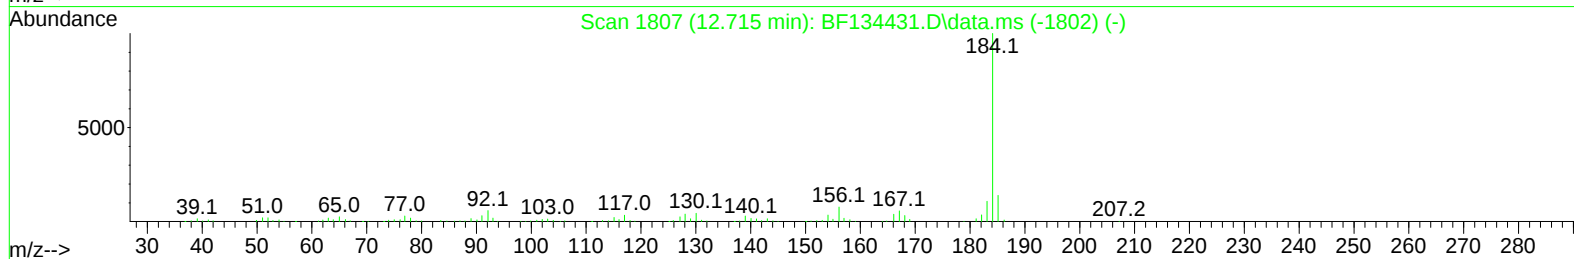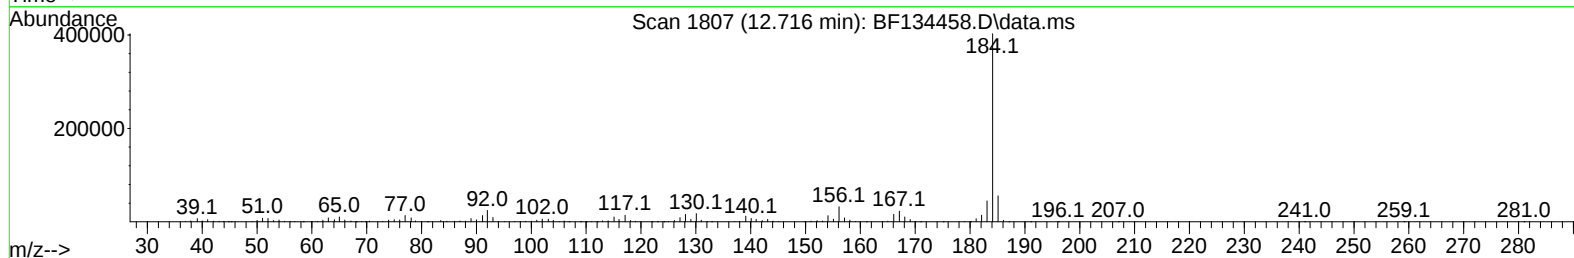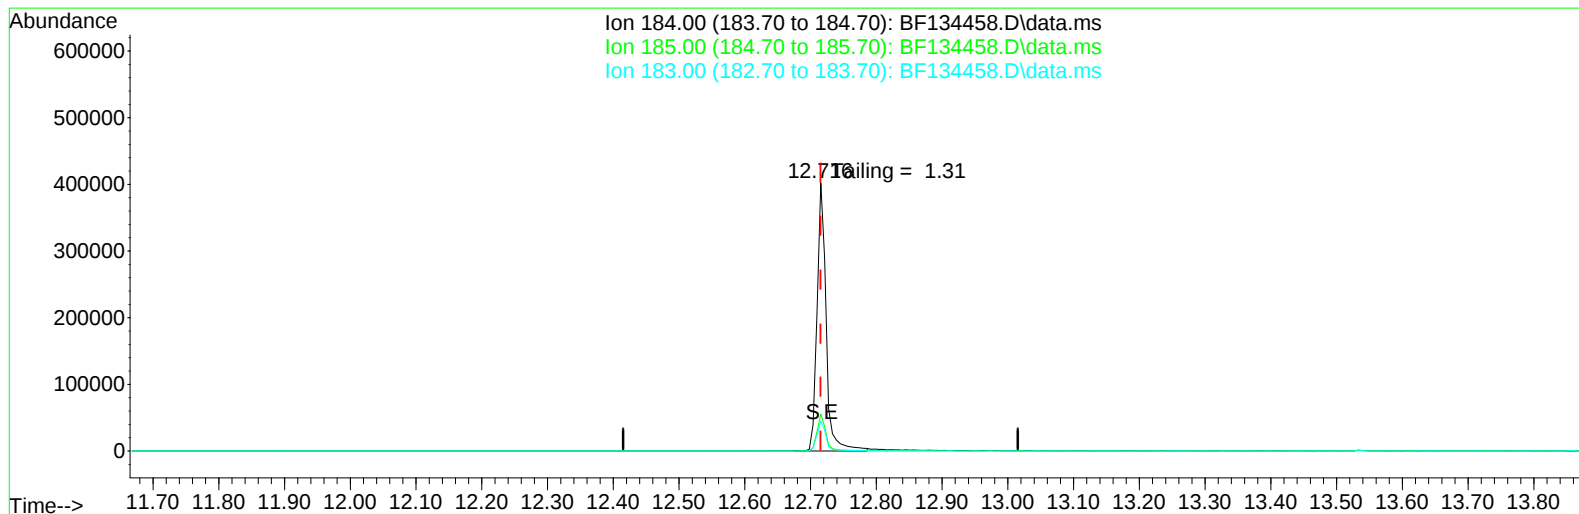

TIC: BF134458.D\data.ms

(77) Benzidine

12.716min (+ 0.001) 245127.37 ng

response 298336

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.80
183.00	10.80	11.12
0.00	0.00	0.00