

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072523\
 Data File : BF134460.D
 Acq On : 25 Jul 2023 13:21
 Operator : CG\JU
 Sample : PB154085BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 PB154085BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BF134460.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	2.175	10	15	22	rVB	31009	45420	1.60%	0.292%
2	5.481	573	577	595	rBV	2243414	2124490	74.73%	13.646%
3	6.481	742	747	750	rBV	2131539	2056774	72.34%	13.211%
4	6.834	803	807	815	rBV	396109	351378	12.36%	2.257%
5	7.398	899	903	906	rBV	1480775	1348187	47.42%	8.660%
6	8.110	1020	1024	1037	rBV	509120	419707	14.76%	2.696%
7	9.192	1202	1208	1211	rBV	2740329	2423688	85.25%	15.568%
8	9.869	1319	1323	1327	rBV	689530	532739	18.74%	3.422%
9	10.669	1454	1459	1462	rBV	1947191	1744515	61.36%	11.206%
10	11.363	1573	1577	1586	rBV	705945	594957	20.93%	3.822%
11	12.963	1844	1849	1852	rBV	3058557	2843066	100.00%	18.262%
12	14.027	2026	2030	2038	rVB	550588	543780	19.13%	3.493%
13	15.527	2280	2285	2291	rBV	404521	539392	18.97%	3.465%




Sum of corrected areas: 15568093

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072523\
Data File : BF134460.D
Acq On : 25 Jul 2023 13:21
Operator : CG\JU
Sample : PB154085BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154085BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

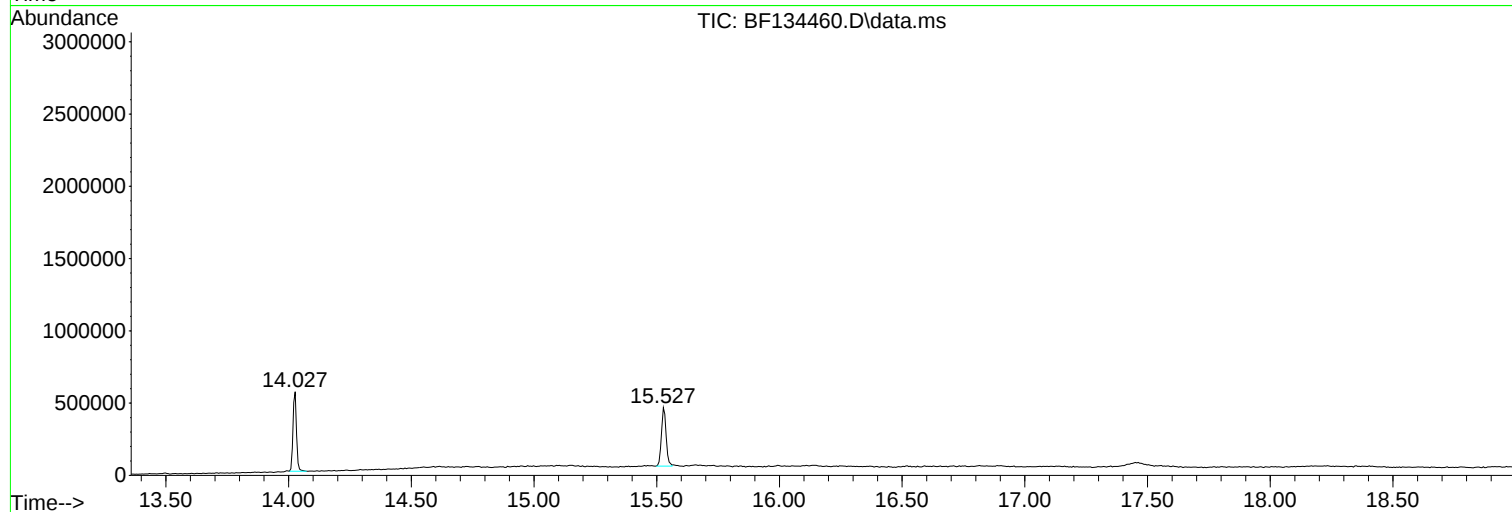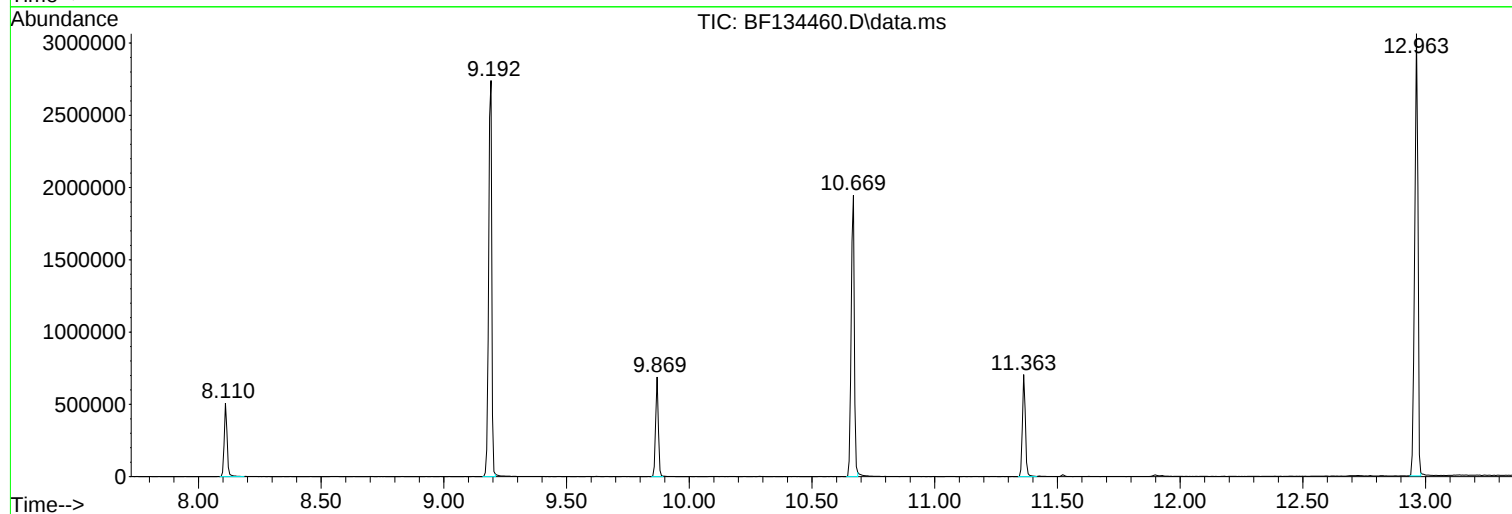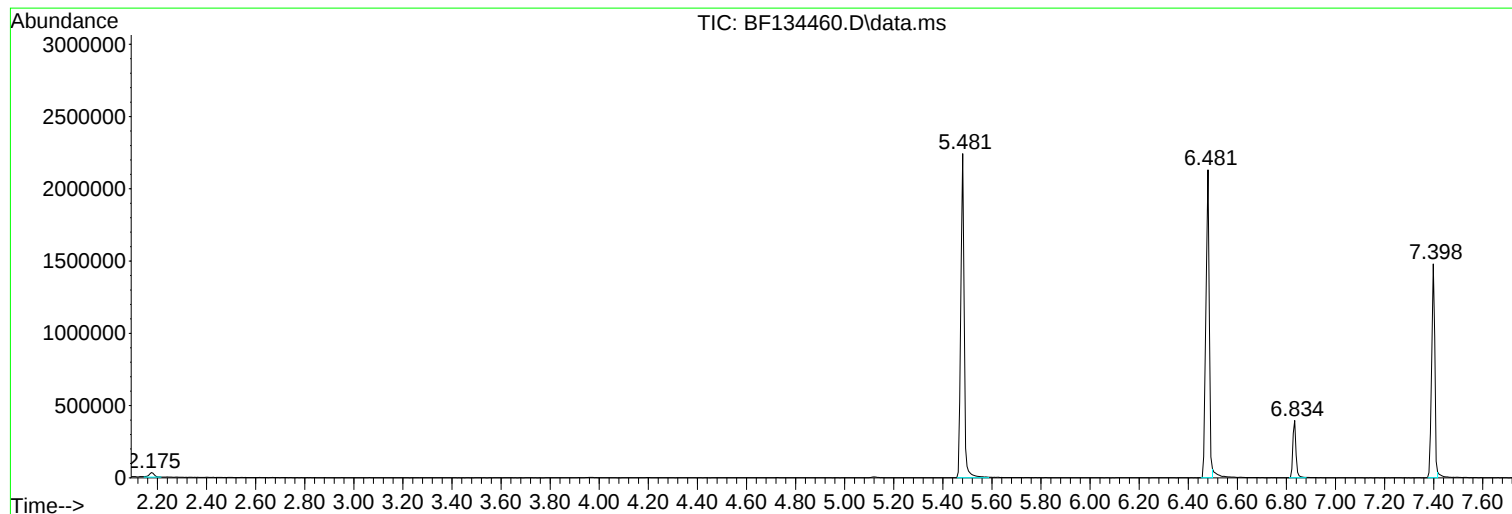

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072523\
Data File : BF134460.D
Acq On : 25 Jul 2023 13:21
Operator : CG\JU
Sample : PB154085BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154085BL










Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Butane, 2-methoxy-2-methyl- Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.175	2.59 ng	45420	1,4-Dichlorobenzene-d4	6.834

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Butane, 2-methoxy-2-methyl-	102	C6H14O	000994-05-8	78
2			3-Pentanol, 3-methyl-	102	C6H14O	000077-74-7	40
3			Silane, ethyltrimethyl-	102	C5H14Si	003439-38-1	39
4			2,2,4-Trimethyl-3-pentanol	130	C8H18O	005162-48-1	39
5			2-Methyl-5-hexen-3-ol	114	C7H14O	032815-70-6	25

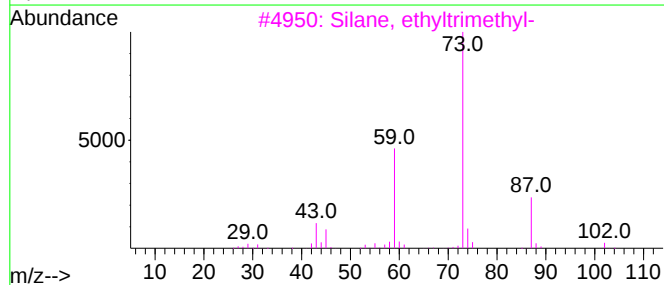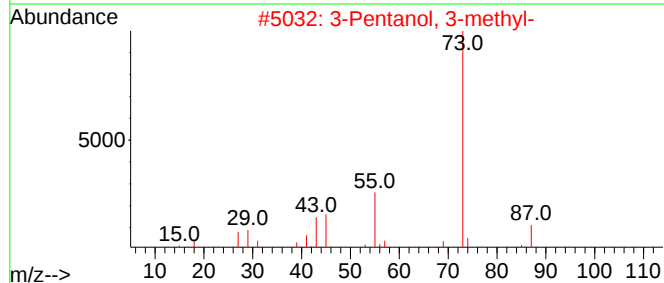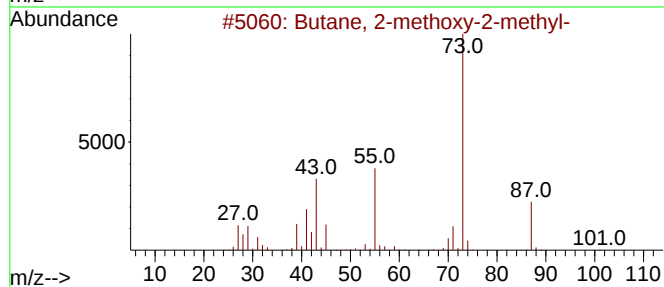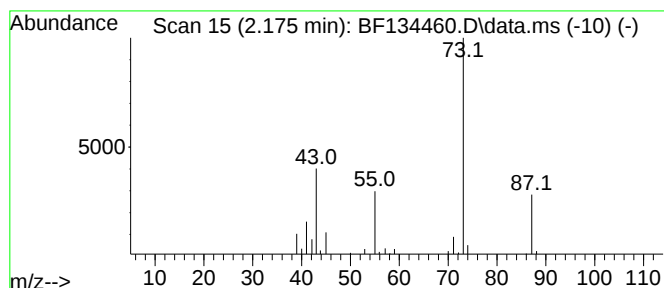

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072523\
Data File : BF134460.D
Acq On : 25 Jul 2023 13:21
Operator : CG\JU
Sample : PB154085BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
PB154085BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Butane, 2-metho...	2.175	2.6	ng	45420	1	6.834	351378	20.0