
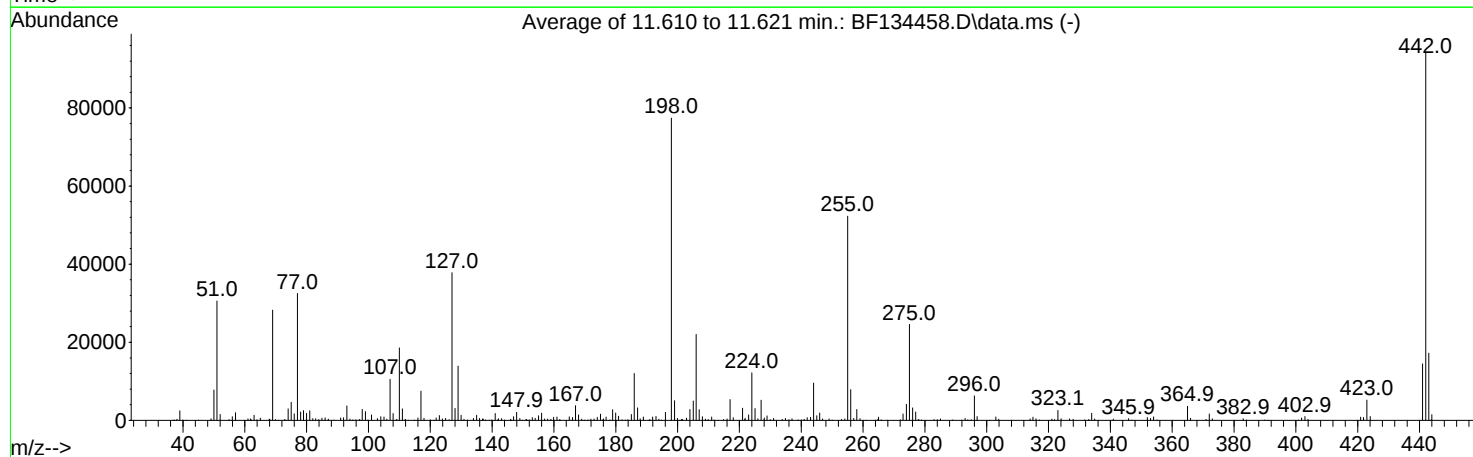


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072523\
Data File : BF134458.D
Acq On : 25 Jul 2023 12:14
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 25 01:46:04 2023

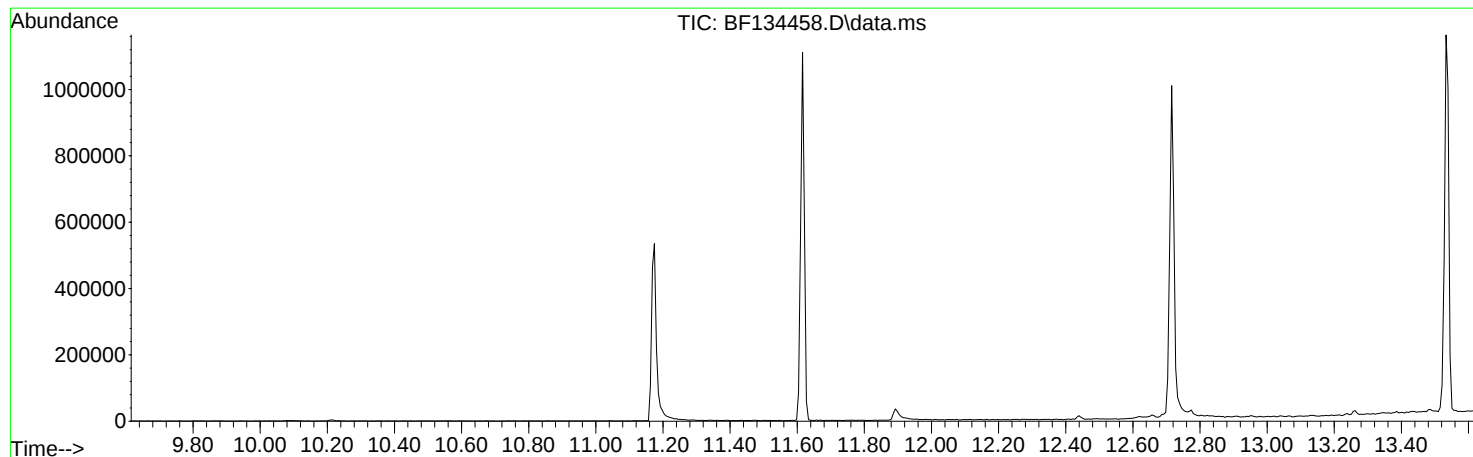

AutoFind: Scans 1619, 1620, 1621; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.5	30575	PASS
68	69	0.00	2	1.2	327	PASS
69	198	0.00	100	36.5	28213	PASS
70	69	0.00	2	0.7	193	PASS
127	198	10	80	48.9	37821	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	77379	PASS
199	198	5	9	6.5	5025	PASS
275	198	10	60	31.8	24579	PASS
365	198	1	100	4.7	3601	PASS
441	198	0.01	100	18.7	14451	PASS
442	442	50	100	100.0	94197	PASS
443	442	15	24	18.3	17219	PASS