


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072618\
Data File : BF107697.D
Acq On : 26 Jul 2018 14:06
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Fri Jul 20 16:29:27 2018

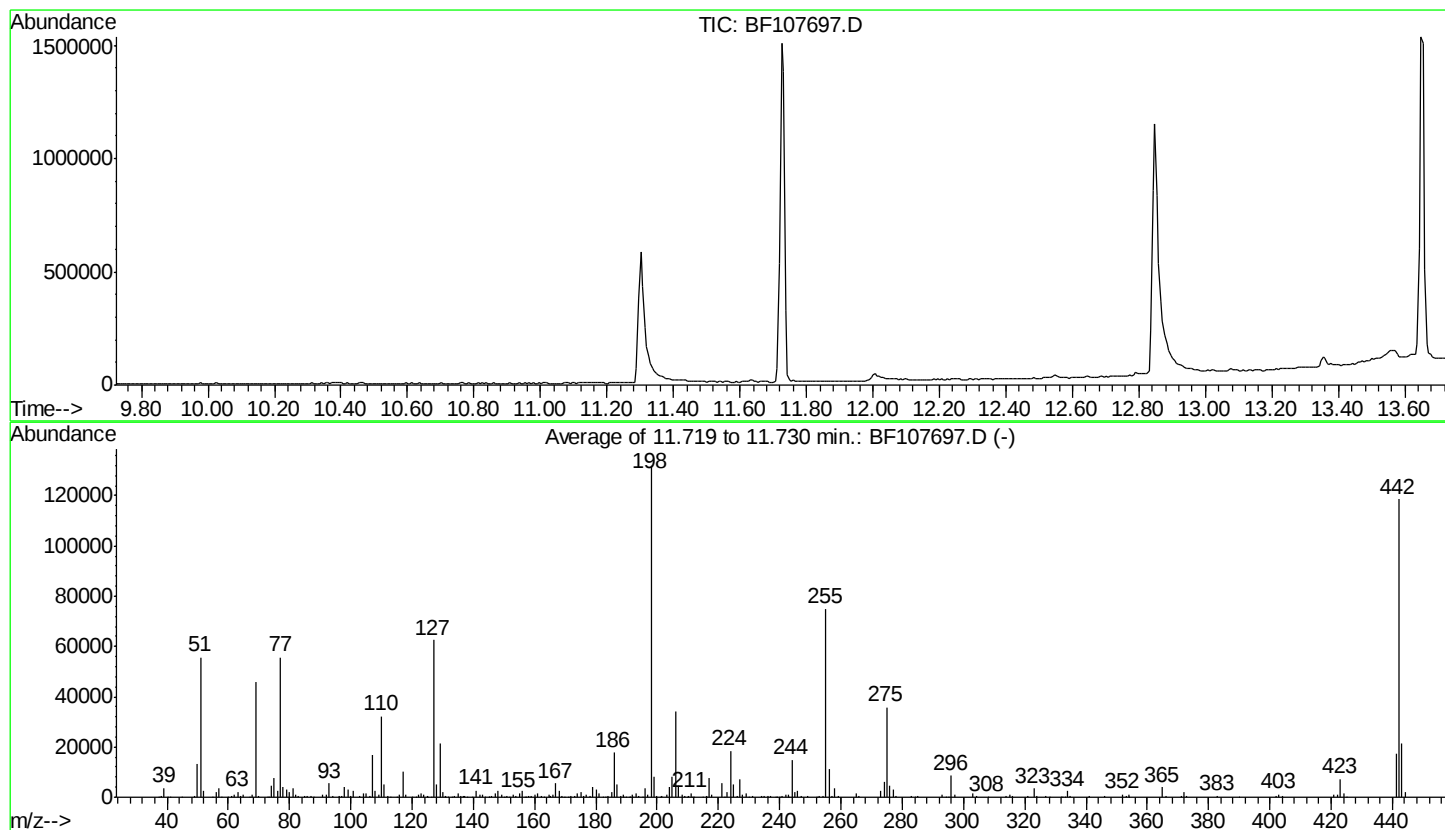

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.3	55774	PASS
68	69	0.00	2	1.8	834	PASS
69	198	0.00	100	34.6	45629	PASS
70	69	0.00	2	0.8	348	PASS
127	198	10	80	47.4	62496	PASS
197	198	0.00	2	0.7	945	PASS
198	198	100	100	100.0	131949	PASS
199	198	5	9	6.4	8416	PASS
275	198	10	60	27.2	35879	PASS
365	198	1	100	3.1	4077	PASS
441	198	0.01	100	13.3	17536	PASS
442	198	50	100	89.8	118512	PASS
443	442	15	24	18.2	21522	PASS