


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF072618\  
 Data File : BF107724.D  
 Acq On : 27 Jul 2018 2:47  
 Operator : JU/SJ  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF072018.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Fri Jul 20 16:29:27 2018

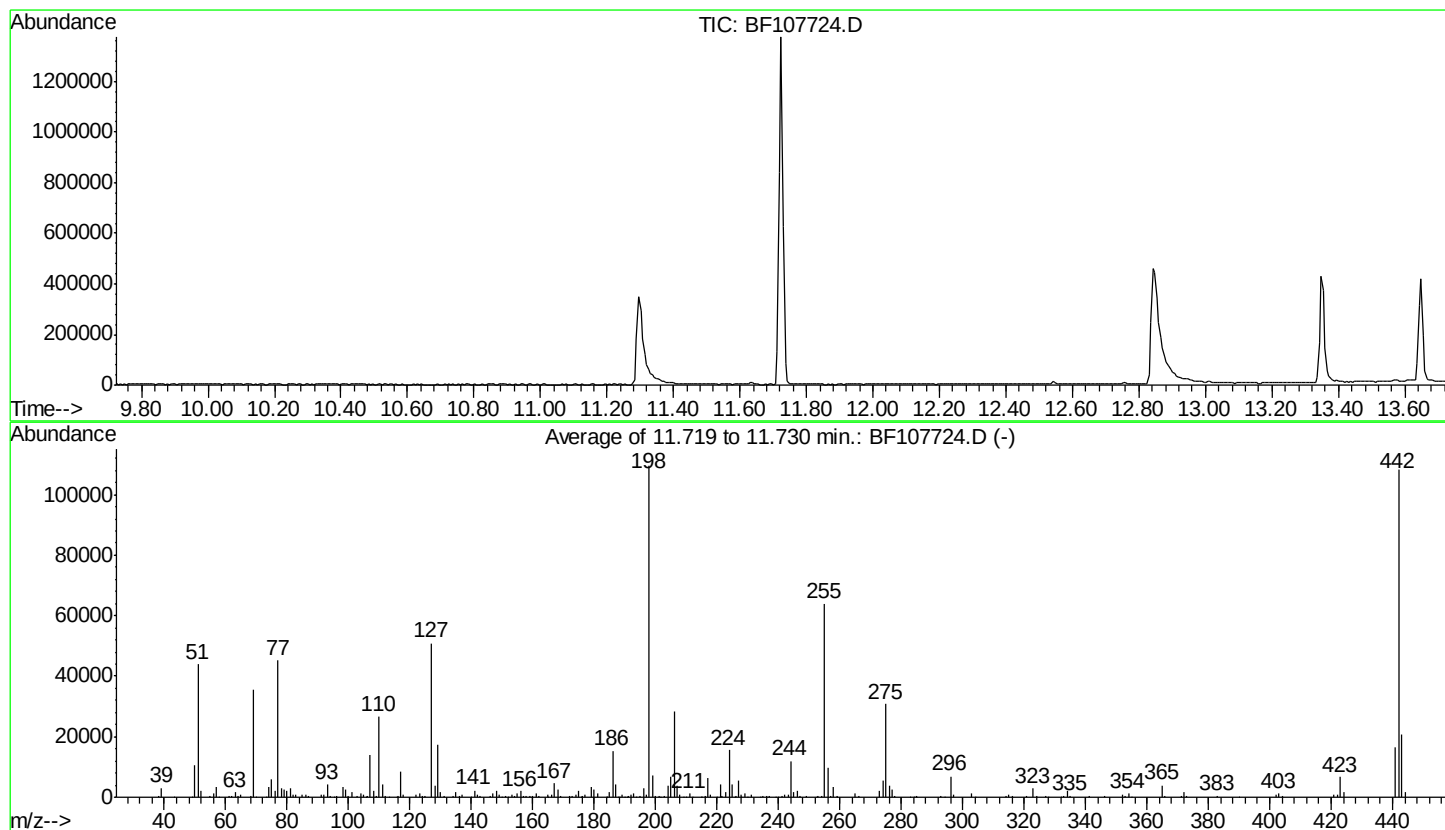

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 40.1      | 43944   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.8       | 635     | PASS             |
| 69          | 198          | 0.00         | 100          | 32.6      | 35689   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 109     | PASS             |
| 127         | 198          | 10           | 80           | 46.4      | 50896   | PASS             |
| 197         | 198          | 0.00         | 2            | 1.0       | 1053    | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 109597  | PASS             |
| 199         | 198          | 5            | 9            | 6.7       | 7323    | PASS             |
| 275         | 198          | 10           | 60           | 28.1      | 30778   | PASS             |
| 365         | 198          | 1            | 100          | 3.5       | 3822    | PASS             |
| 441         | 198          | 0.01         | 100          | 15.0      | 16448   | PASS             |
| 442         | 198          | 50           | 100          | 98.7      | 108136  | PASS             |
| 443         | 442          | 15           | 24           | 19.1      | 20645   | PASS             |