
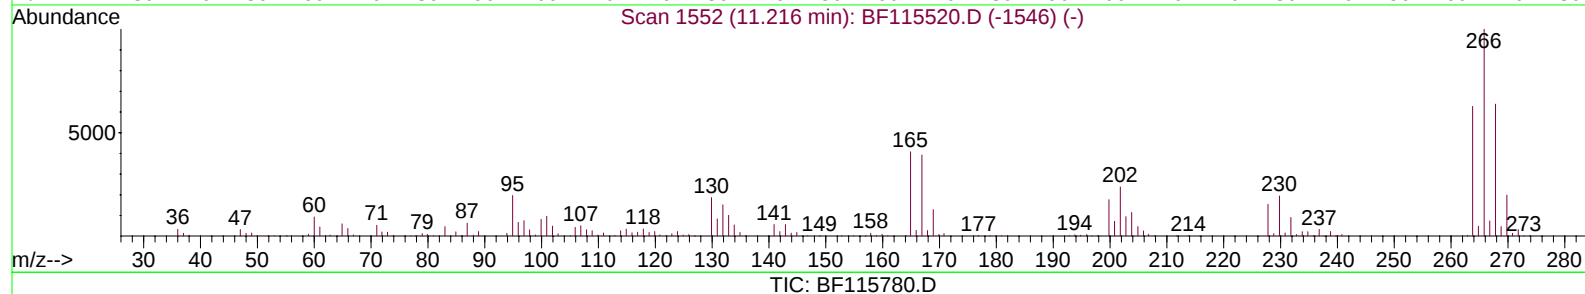
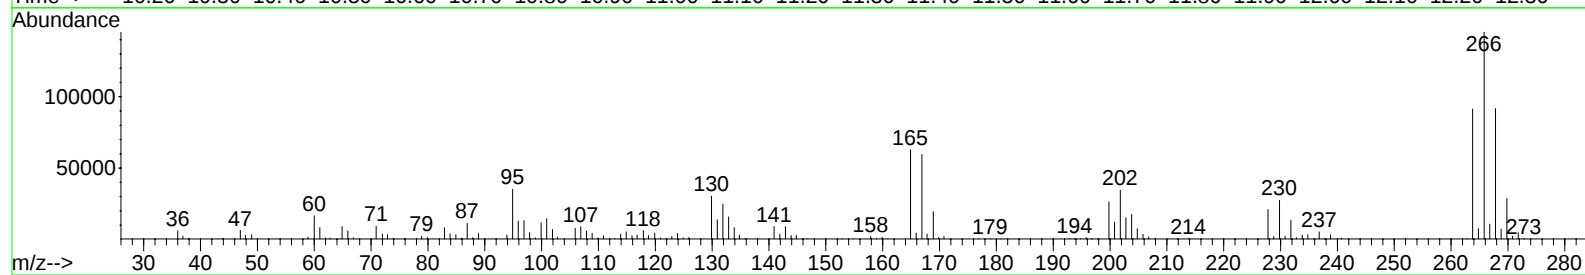


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072619\
Data File : BF115780.D
Acq On : 26 Jul 2019 10:16
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 18:58:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 13:16:07 2019
Response via : Initial Calibration

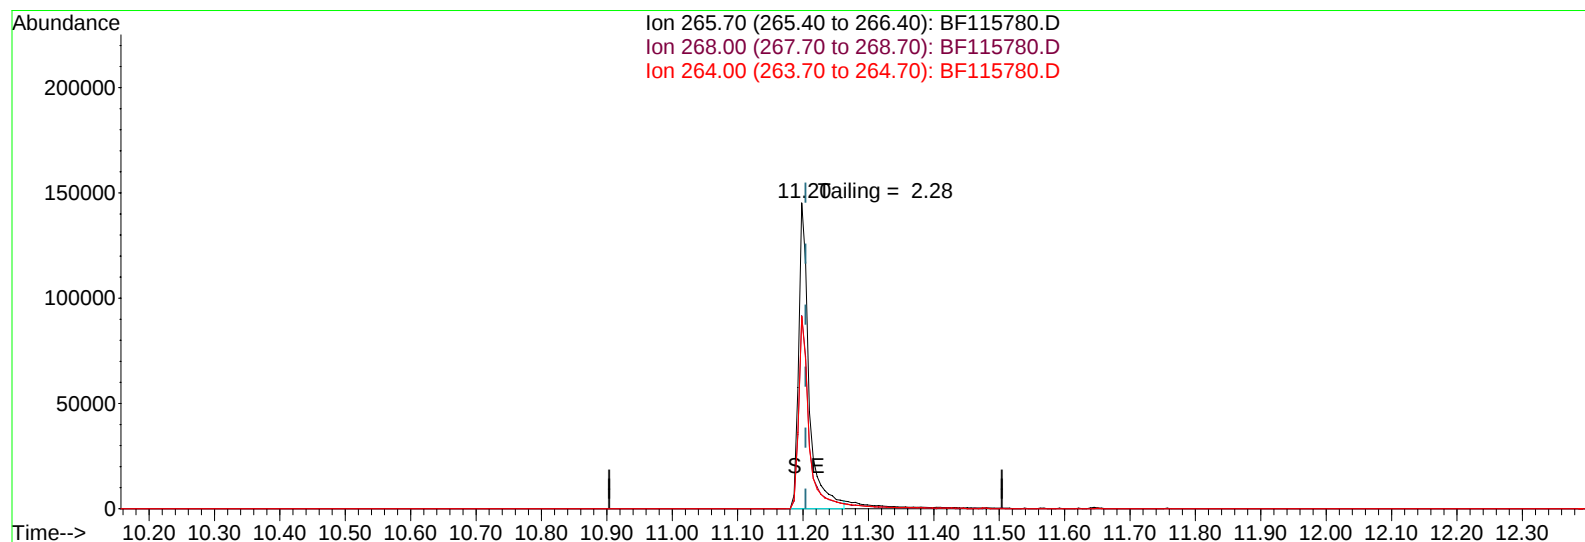

TIC: BF115780.D

(70) Pentachlorophenol (C)




11.198min (-0.006) 33730.06ng

response 172307

Ion	Exp%	Act%
265.70	100	100
268.00	64.00	63.13
264.00	62.50	62.91
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF072619\
Data File : BF115780.D
Acq On : 26 Jul 2019 10:16
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 18:58:07 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 13:16:07 2019
Response via : Initial Calibration

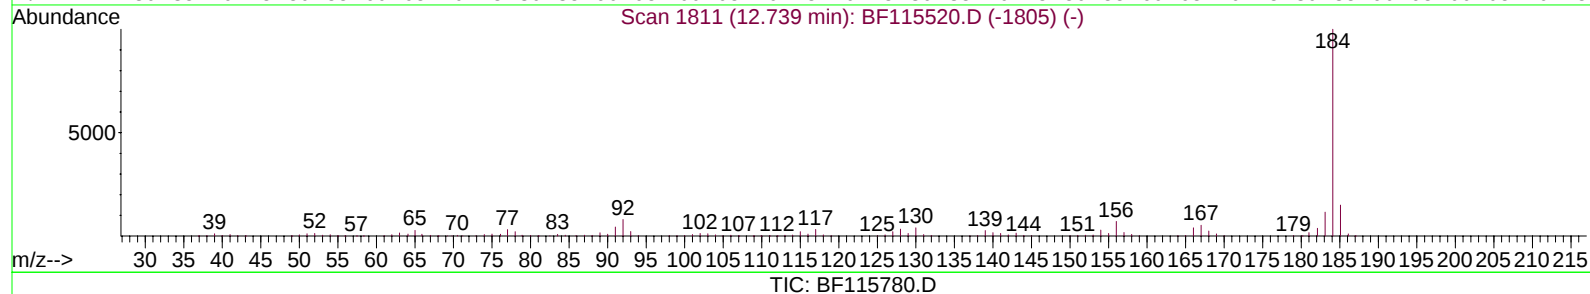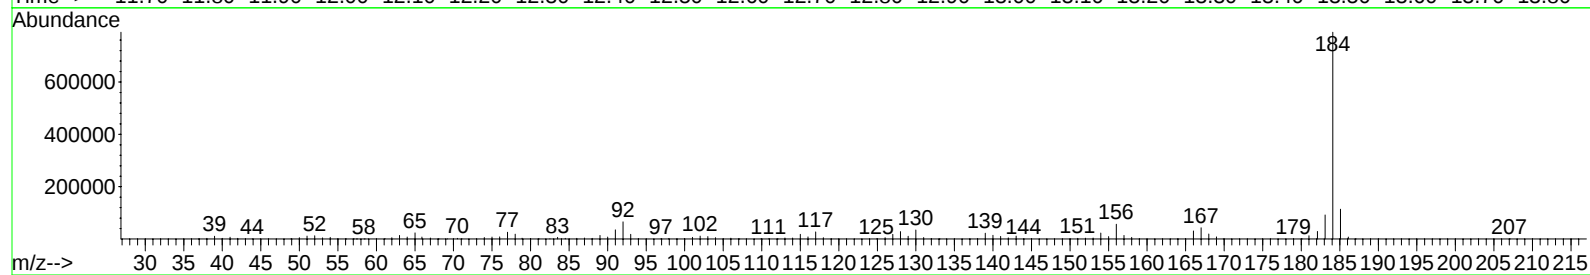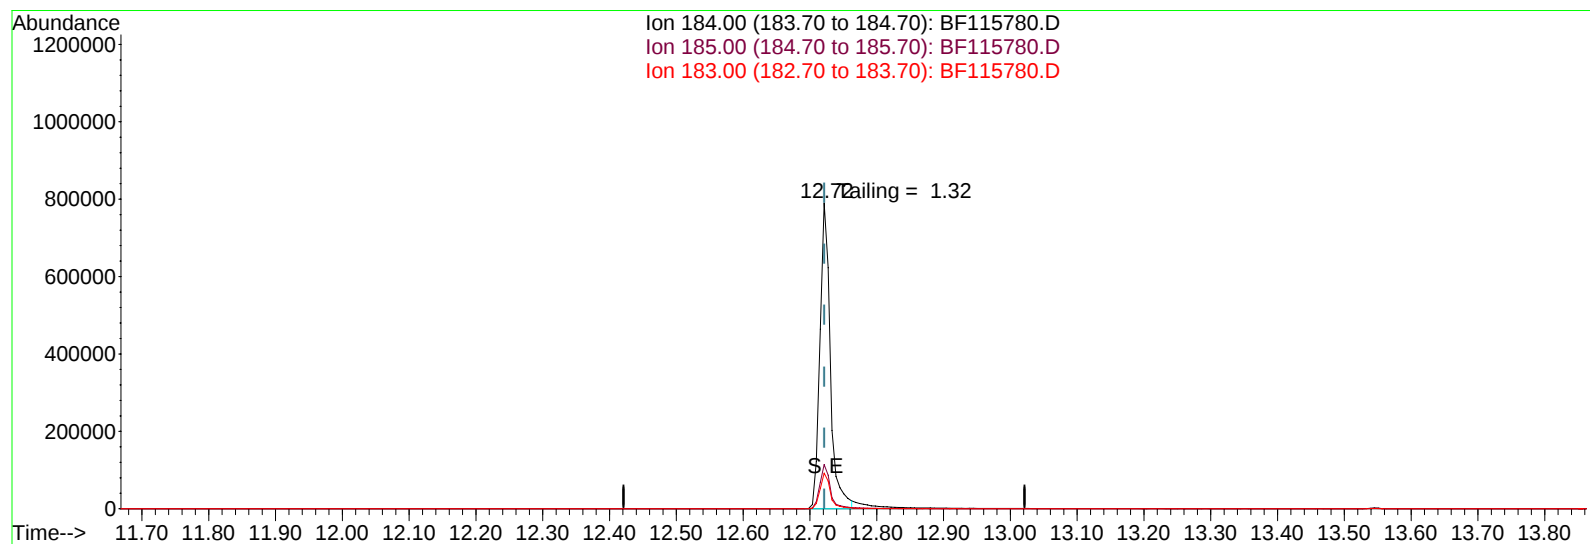

(77) Benzidine

12.721min (-0.000) 0.00ng

response 897925

Ion	Exp%	Act%
184.00	100	100
185.00	15.60	14.44
183.00	11.50	11.66
0.00	0.00	0.00