


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072619\
 Data File : BF115780.D
 Acq On : 26 Jul 2019 10:16
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 29 16:38:26 2019

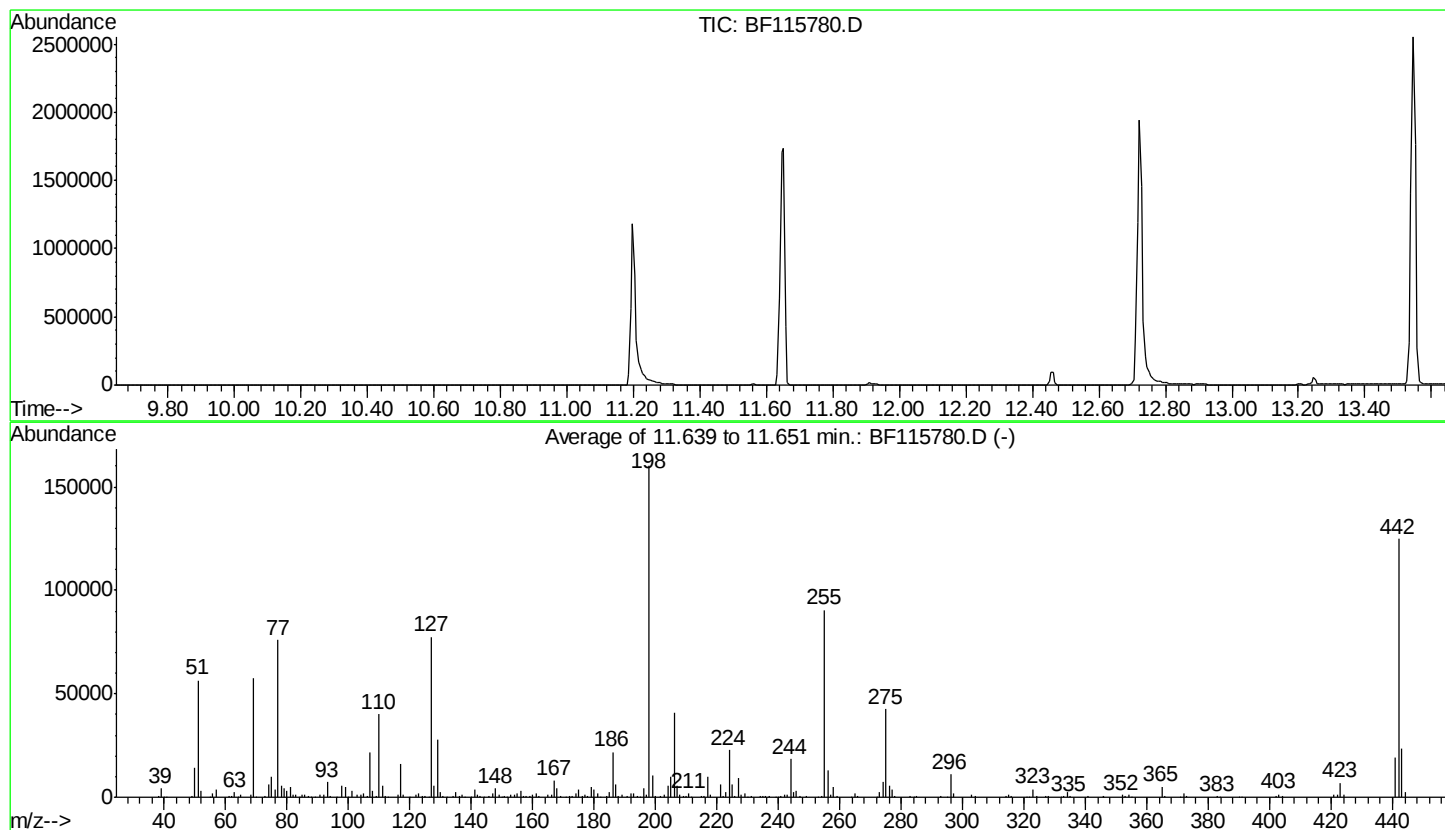

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	35.2	56402	PASS
68	69	0.00	2	1.7	982	PASS
69	198	0.00	100	36.0	57682	PASS
70	69	0.00	2	0.4	248	PASS
127	198	10	80	48.4	77653	PASS
197	198	0.00	2	0.6	955	PASS
198	198	100	100	100.0	160288	PASS
199	198	5	9	6.7	10803	PASS
275	198	10	60	26.6	42571	PASS
365	198	1	100	3.2	5144	PASS
441	198	0.01	100	12.1	19447	PASS
442	198	50	100	77.8	124736	PASS
443	442	15	24	18.9	23585	PASS