


Data Path : Z:\SVOASRV\HPCHEM1\BNA\_F\DATA\BF072619\  
 Data File : BF115791.D  
 Acq On : 26 Jul 2019 16:55  
 Operator : HP/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_F  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_F\METHODS\8270-BF071219.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Mon Jul 29 16:38:26 2019

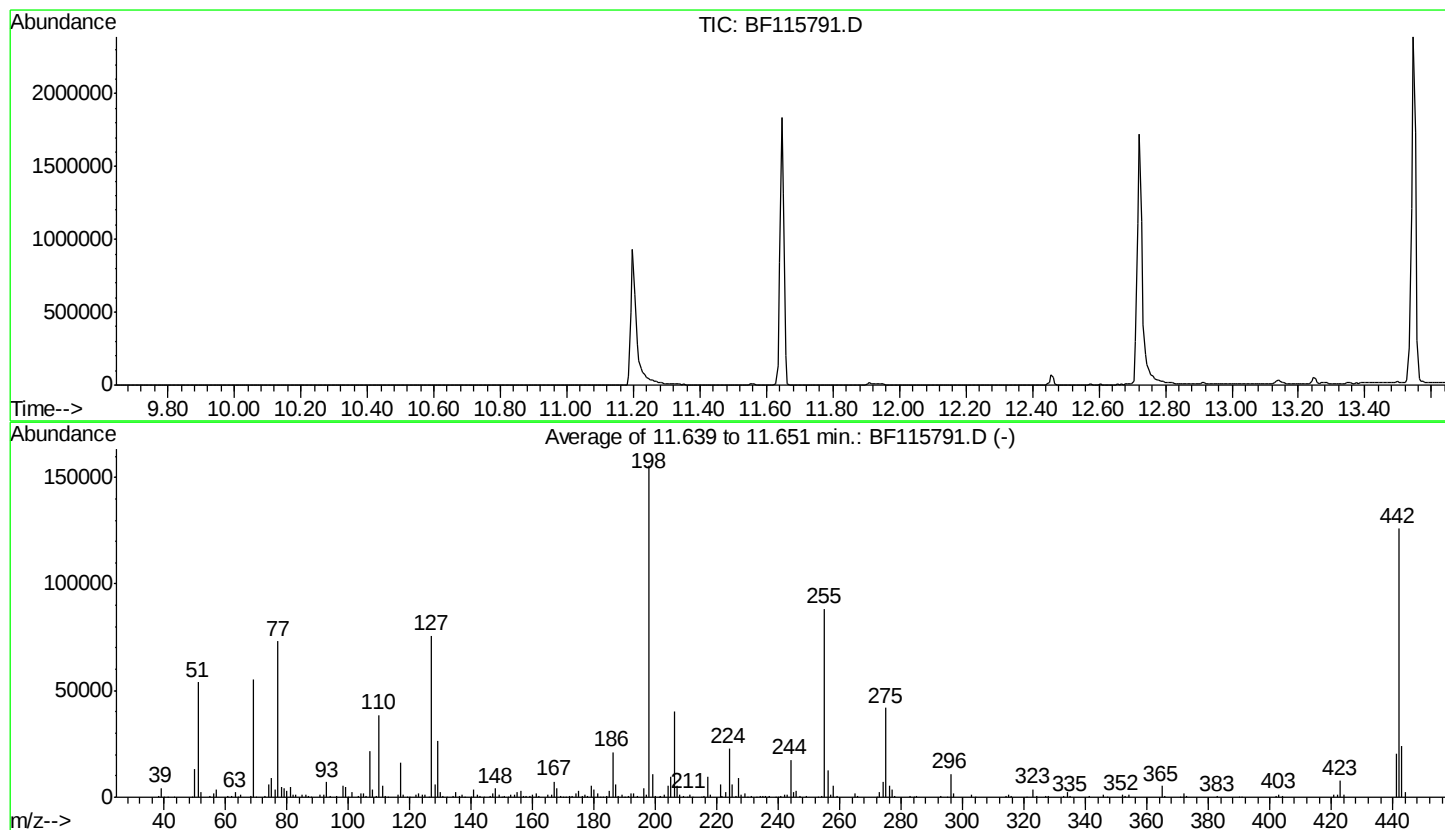

AutoFind: Scans 1624, 1625, 1626; Background Corrected with Scan 1619

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 34.6      | 53861   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 877     | PASS             |
| 69          | 198          | 0.00         | 100          | 35.6      | 55413   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.3       | 150     | PASS             |
| 127         | 198          | 10           | 80           | 48.7      | 75757   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.6       | 980     | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 155544  | PASS             |
| 199         | 198          | 5            | 9            | 6.9       | 10659   | PASS             |
| 275         | 198          | 10           | 60           | 26.9      | 41776   | PASS             |
| 365         | 198          | 1            | 100          | 3.3       | 5185    | PASS             |
| 441         | 198          | 0.01         | 100          | 13.2      | 20482   | PASS             |
| 442         | 198          | 50           | 100          | 80.9      | 125824  | PASS             |
| 443         | 442          | 15           | 24           | 19.3      | 24254   | PASS             |