
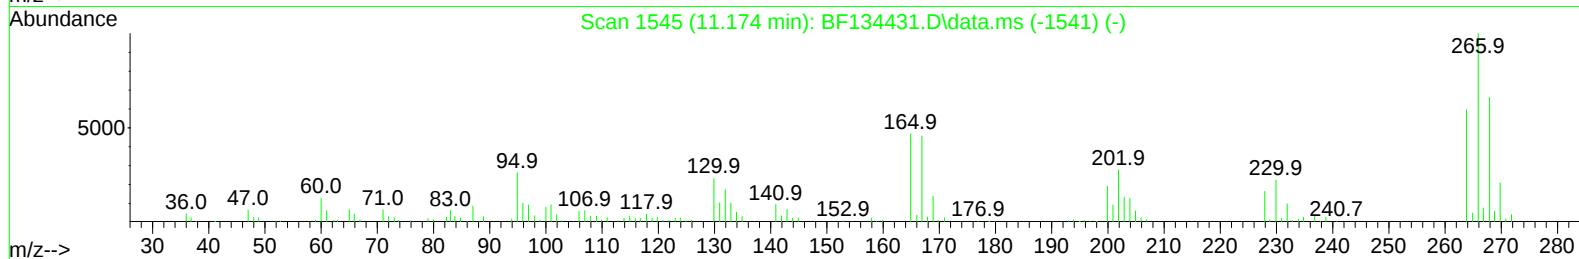
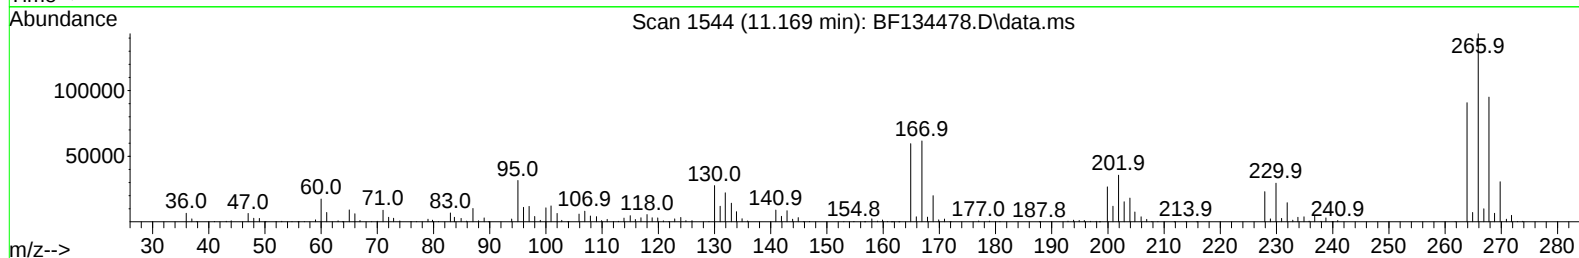


Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072623\  
Data File : BF134478.D  
Acq On : 26 Jul 2023 12:51  
Operator : CG\JU  
Sample : DFTPP  
Misc :  
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 14:32:23 2023  
Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072423.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
QLast Update : Tue Jul 25 01:46:04 2023  
Response via : Initial Calibration

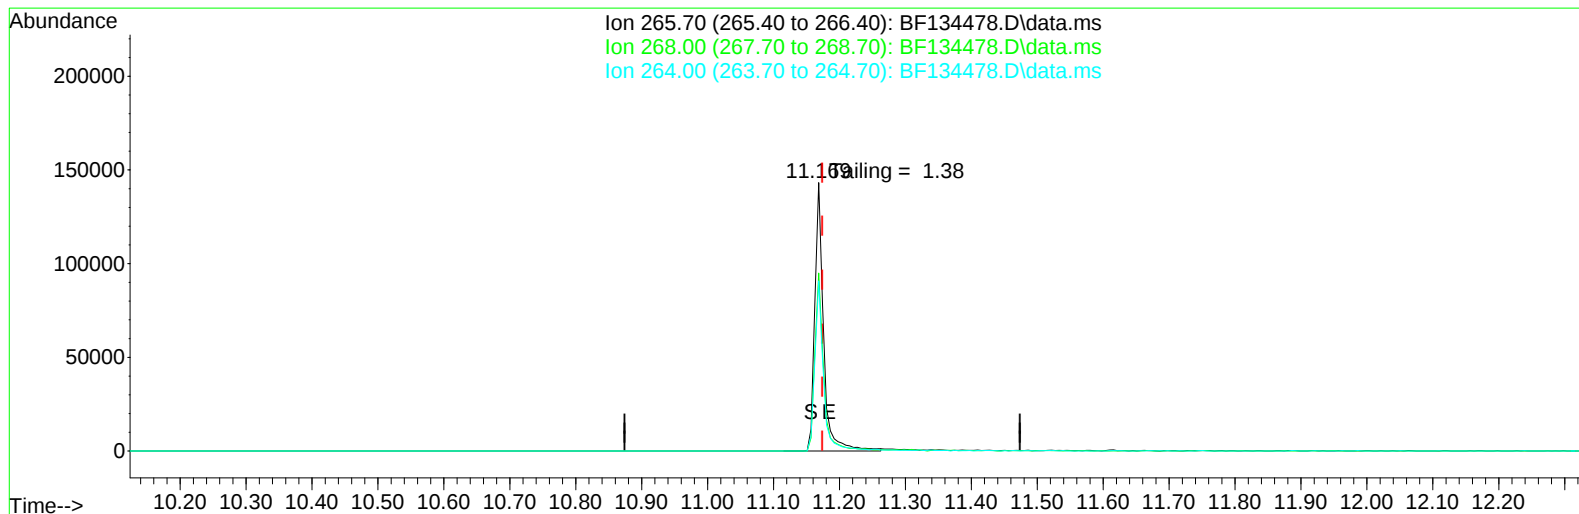

TIC: BF134478.D\data.ms

**(70) Pentachlorophenol (C)**




11.169min (-0.005) 310598.17 ng

response 136698

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 265.70 | 100.00 | 100.00 |
| 268.00 | 66.10  | 66.31  |
| 264.00 | 59.70  | 63.37  |
| 0.00   | 0.00   | 0.00   |

Data Path : Z:\svoasrv\HPCHEM1\BNA\_F\Data\BF072623\  
 Data File : BF134478.D  
 Acq On : 26 Jul 2023 12:51  
 Operator : CG\JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 26 14:32:23 2023  
 Quant Method : Z:\svoasrv\HPCHEM1\BNA\_F\Methods\8270-BF072423.M  
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 QLast Update : Tue Jul 25 01:46:04 2023  
 Response via : Initial Calibration

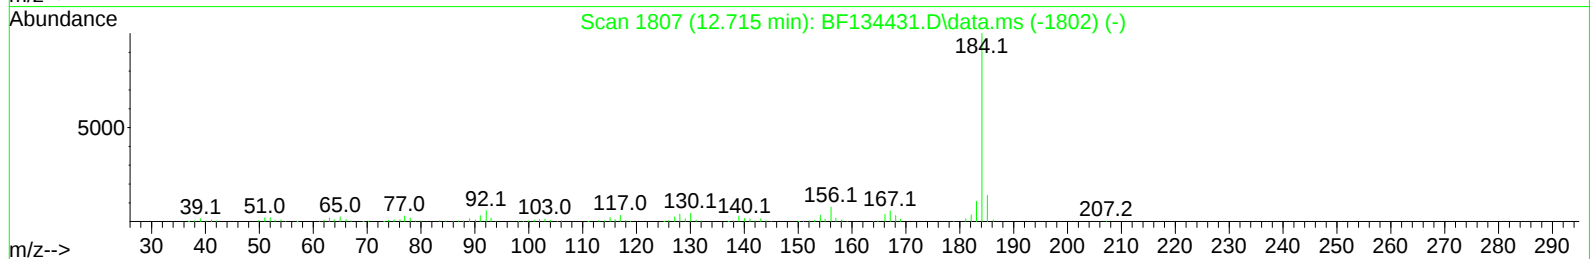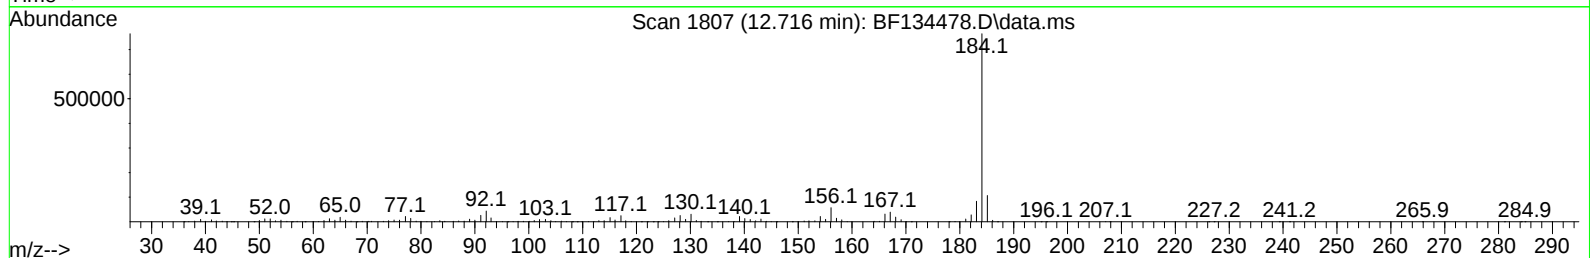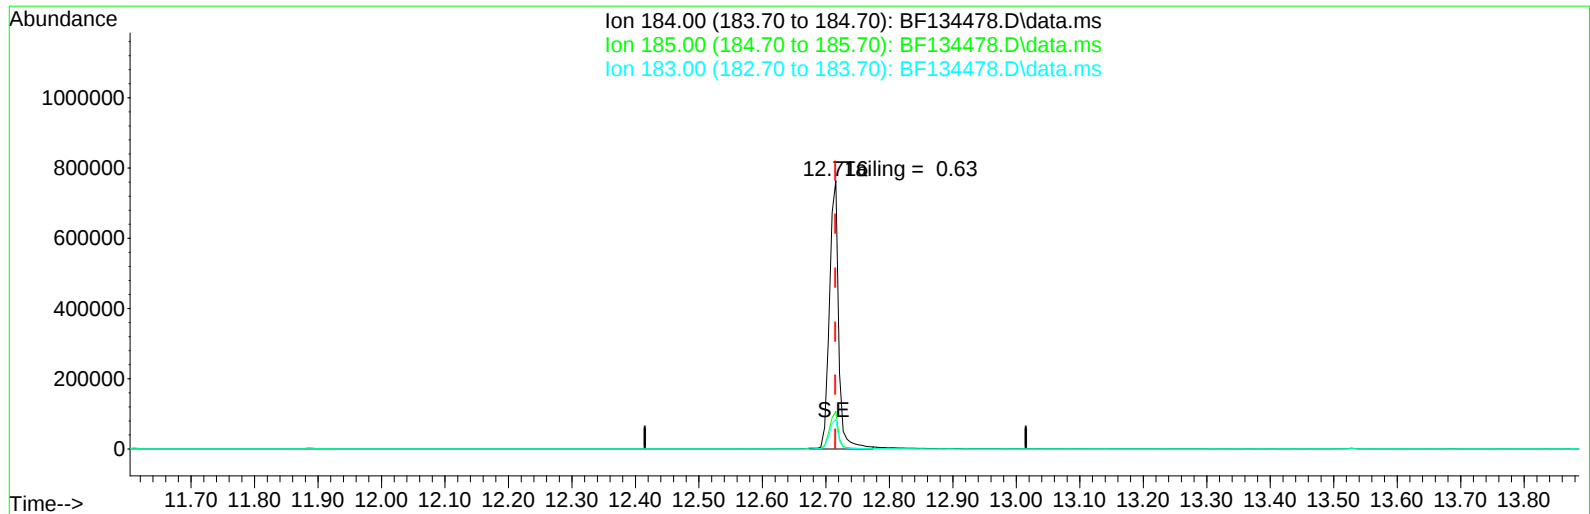

TIC: BF134478.D\data.ms

**(77) Benzidine**

12.716min (+ 0.001) 80695.04 ng

response 790858

| Ion    | Exp%   | Act%   |
|--------|--------|--------|
| 184.00 | 100.00 | 100.00 |
| 185.00 | 14.00  | 13.96  |
| 183.00 | 10.80  | 10.93  |
| 0.00   | 0.00   | 0.00   |