
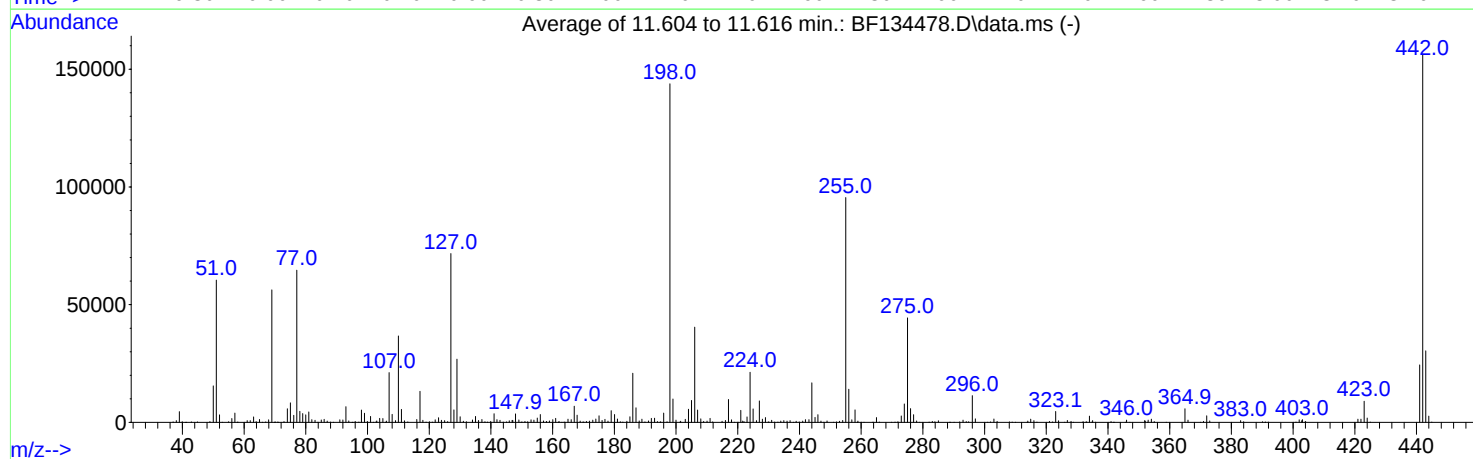


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072623\
 Data File : BF134478.D
 Acq On : 26 Jul 2023 12:51
 Operator : CG\JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Jul 27 12:16:03 2023

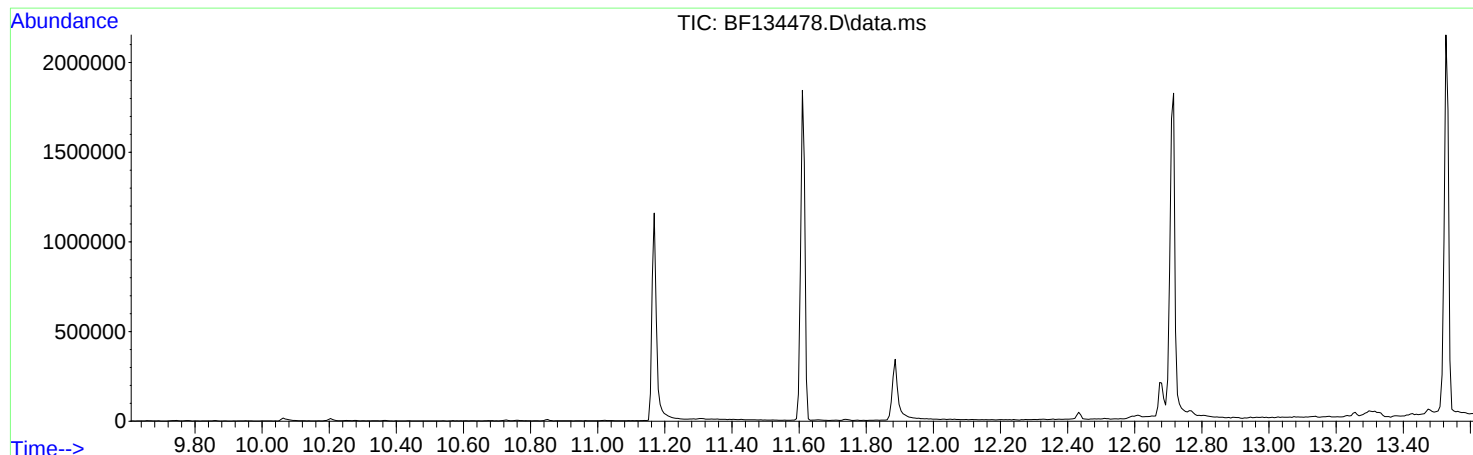




AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	60403	PASS
68	69	0.00	2	1.9	1086	PASS
69	198	0.00	100	39.1	56290	PASS
70	69	0.00	2	0.4	219	PASS
127	198	10	80	49.9	71747	PASS
197	198	0.00	2	0.2	297	PASS
198	198	100	100	100.0	143859	PASS
199	198	5	9	6.9	9912	PASS
275	198	10	60	30.9	44387	PASS
365	198	1	100	4.0	5809	PASS
441	198	0.01	100	17.0	24415	PASS
442	442	50	100	100.0	156272	PASS
443	442	15	24	19.5	30411	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072623\
Data File : BF134478.D
Acq On : 26 Jul 2023 12:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 26 14:32:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

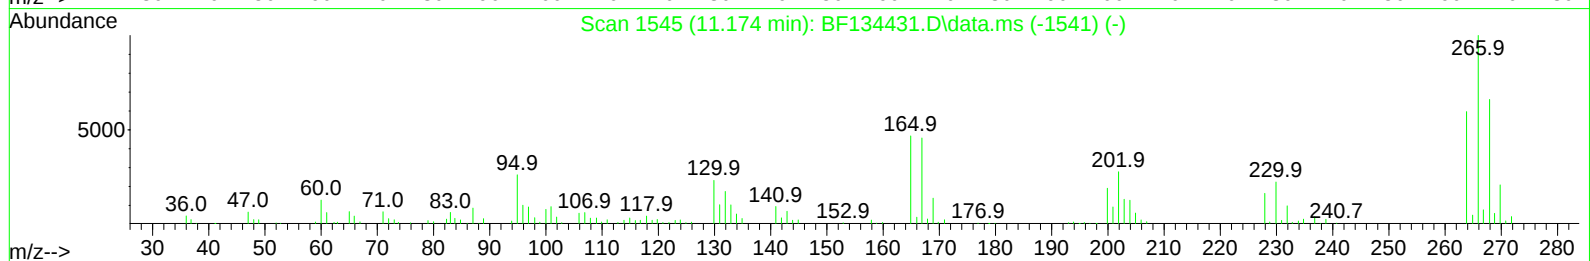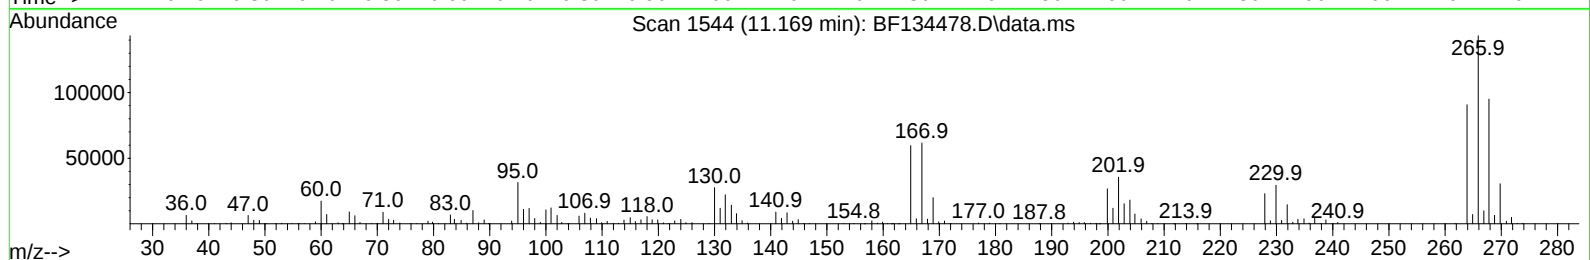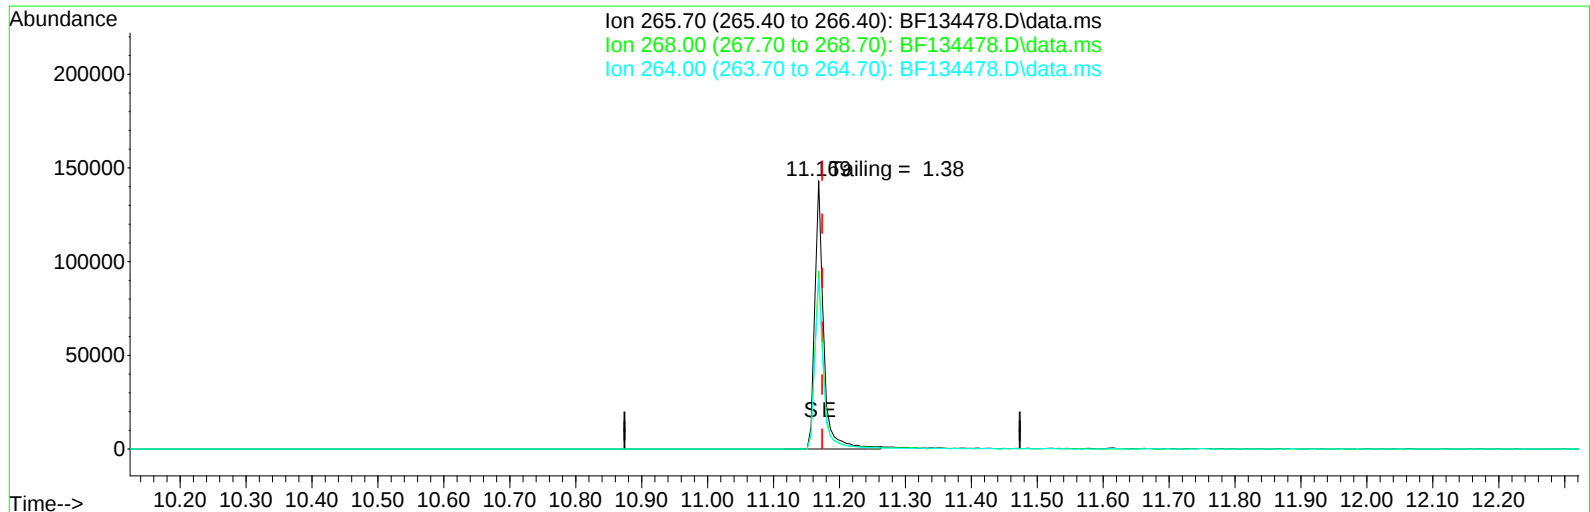

TIC: BF134478.D\data.ms

(70) Pentachlorophenol (C)

11.169min (-0.005) 310598.17 ng




response 136698

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	66.31
264.00	59.70	63.37
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072623\
Data File : BF134478.D
Acq On : 26 Jul 2023 12:51
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 26 14:32:23 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

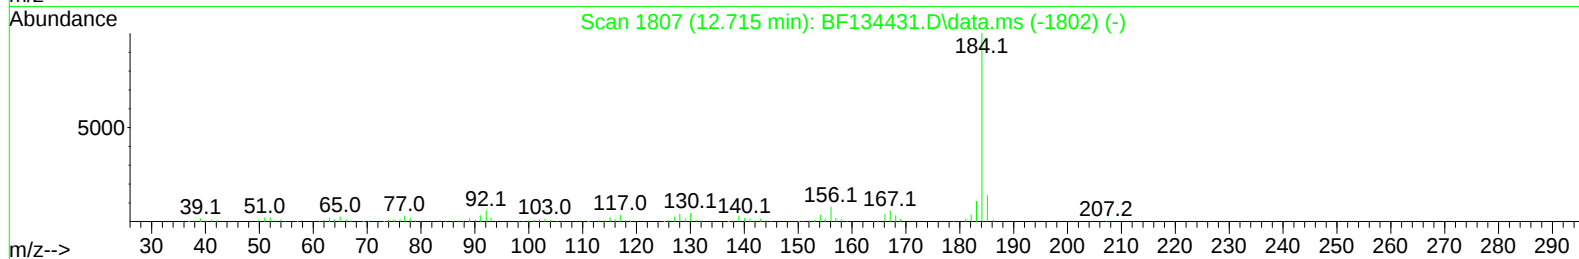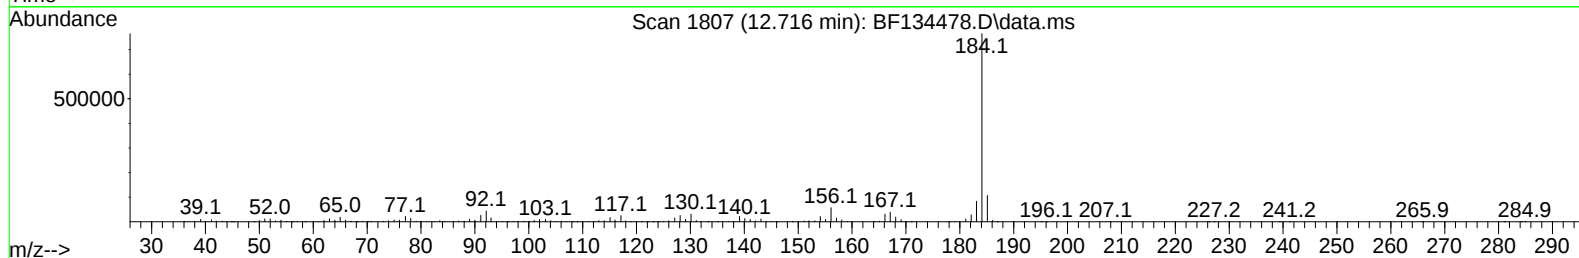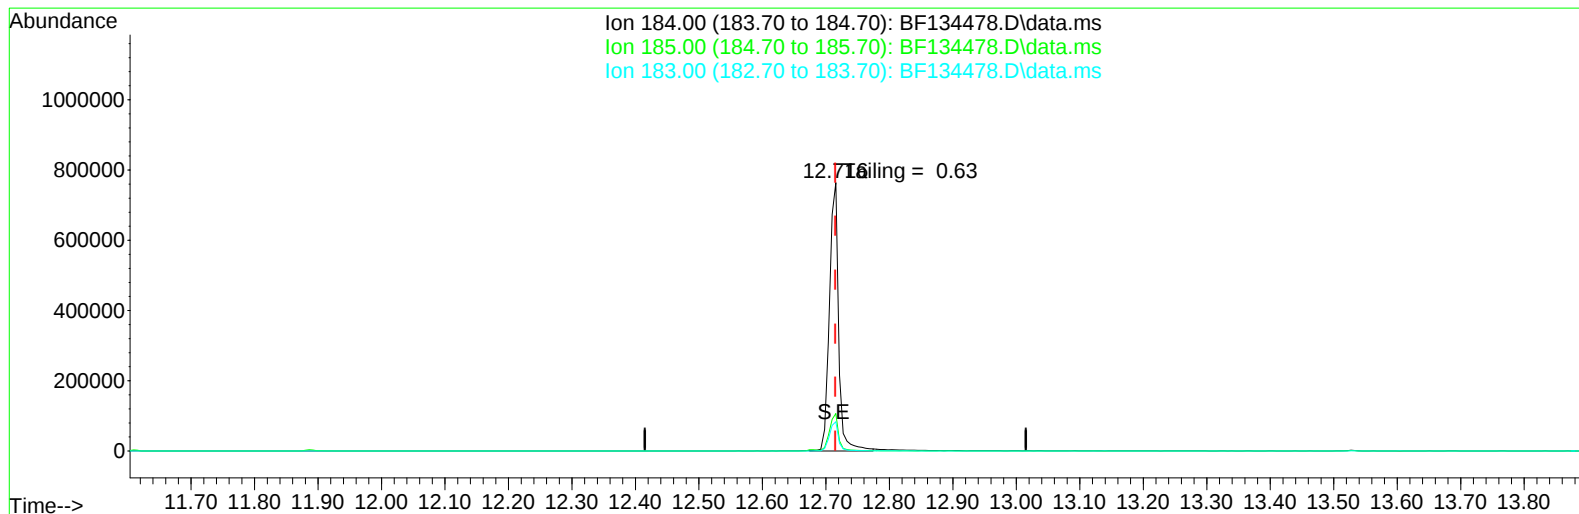

TIC: BF134478.D\data.ms

(77) Benzidine

12.716min (+ 0.001) 80695.04 ng

response 790858

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.96
183.00	10.80	10.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/26/2023	BNA_F	<u>BF134478.D</u>
Compound Name	Response	Retention Time
DDT	367314	13.527
DDD	5233	13.257
DDE	150	12.898
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
5383	372697	1.44

Instrument :
BNA_F
ClientSampleId :
DFTPP