


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072718\
 Data File : BF107742.D
 Acq On : 27 Jul 2018 13:29
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF072018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Jul 20 16:29:27 2018

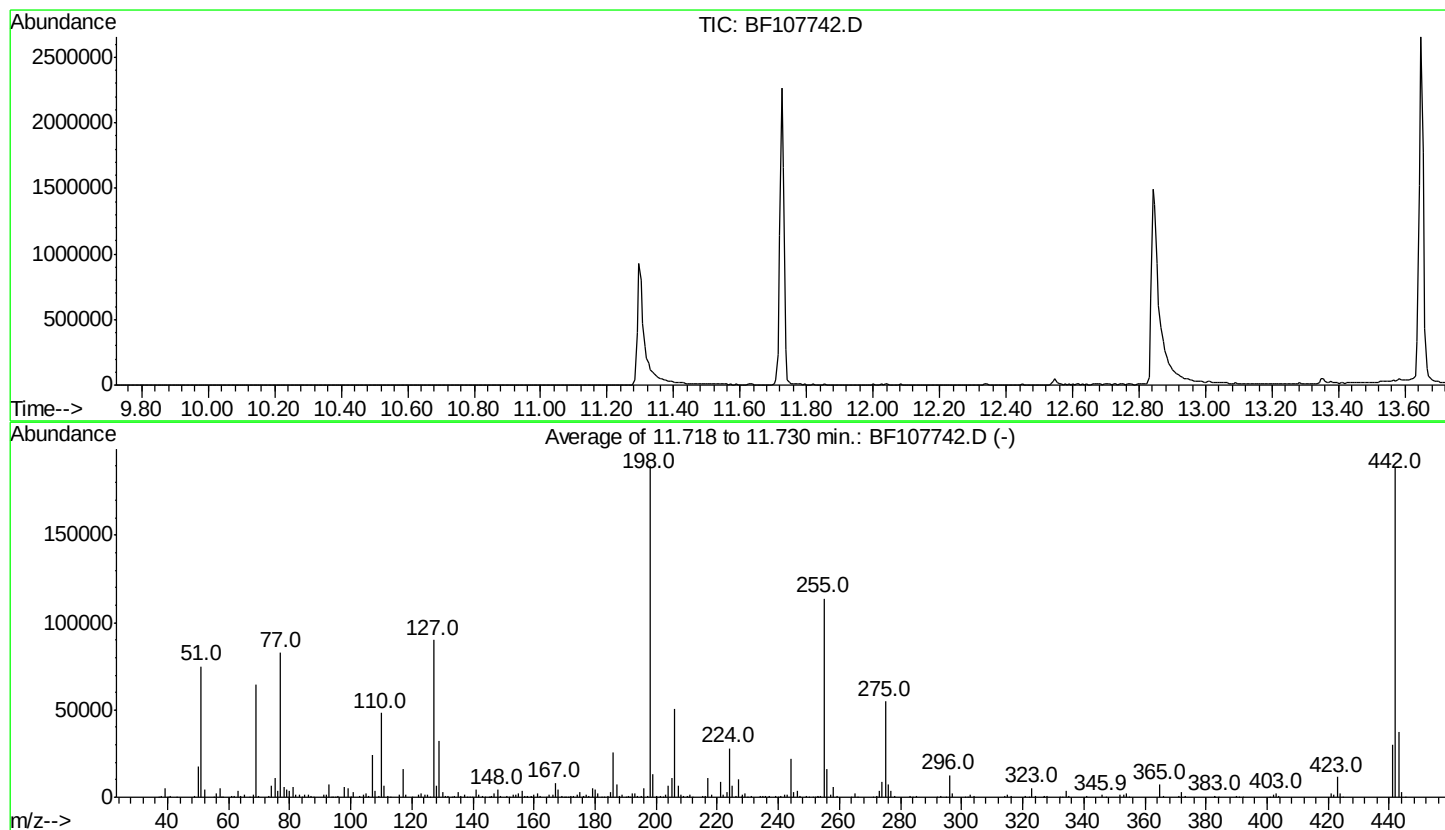

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1589

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	39.6	75090	PASS
68	69	0.00	2	1.9	1234	PASS
69	198	0.00	100	33.8	64216	PASS
70	69	0.00	2	0.7	469	PASS
127	198	10	80	47.4	89941	PASS
197	198	0.00	2	0.5	892	PASS
198	198	100	100	100.0	189853	PASS
199	198	5	9	6.9	13006	PASS
275	198	10	60	28.9	54906	PASS
365	198	1	100	3.7	7080	PASS
441	198	0.01	100	15.9	30124	PASS
442	198	50	100	99.8	189410	PASS
443	442	15	24	19.7	37302	PASS