

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072719\
 Data File : BF115824.D
 Acq On : 27 Jul 2019 12:16
 Operator : HP/JU
 Sample : K3992-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 55-ST-19

Quant Time: Jul 29 02:00:48 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Jul 25 13:16:07 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	6.87	152	144179	20.00	ng	0.00
21) Naphthalene-d8	8.15	136	542067	20.00	ng	0.00
39) Acenaphthene-d10	9.90	164	299967	20.00	ng	0.00
64) Phenanthrene-d10	11.39	188	523240	20.00	ng	0.00
76) Chrysene-d12	14.03	240	375472	20.00	ng	0.00
87) Perylene-d12	15.50	264	365352	20.00	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.49	112	361301	40.99	ng	0.00
7) Phenol-d6	6.49	99	286568	25.62	ng	-0.01
23) Nitrobenzene-d5	7.43	82	895745	96.09	ng	0.00
42) 2,4,6-Tribromophenol	10.70	330	289407	82.66	ng	0.00
45) 2-Fluorobiphenyl	9.23	172	1600332	93.38	ng	0.00
79) Terphenyl-d14	12.97	244	1658160	81.49	ng	0.00
Target Compounds						
50) Dimethylphthalate	9.62	163	135374	5.998	ng	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF072719\
Data File : BF115824.D
Acq On : 27 Jul 2019 12:16
Operator : HP/JU
Sample : K3992-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
55-ST-19

Quant Time: Jul 29 02:00:48 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF071219.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 25 13:16:07 2019
Response via : Initial Calibration

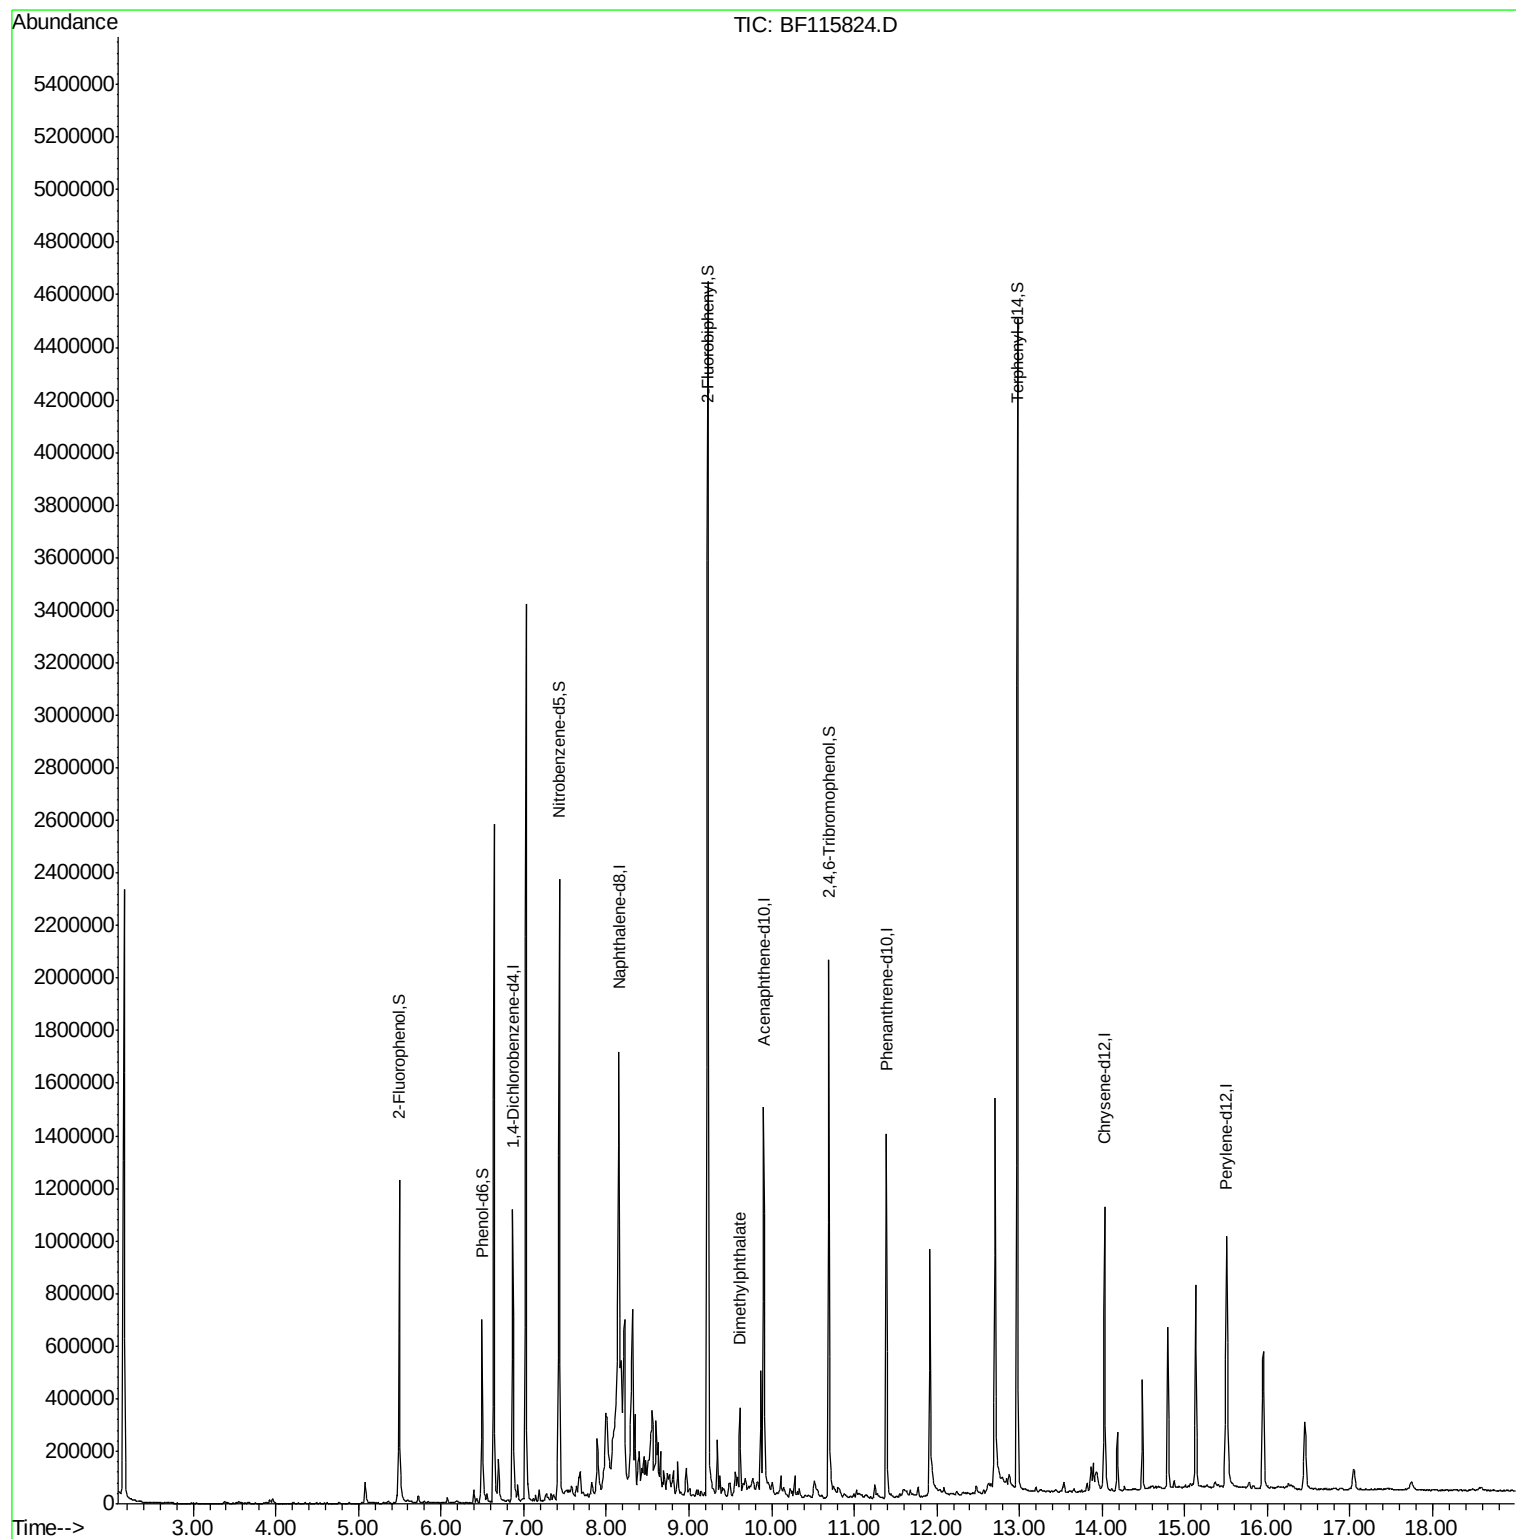

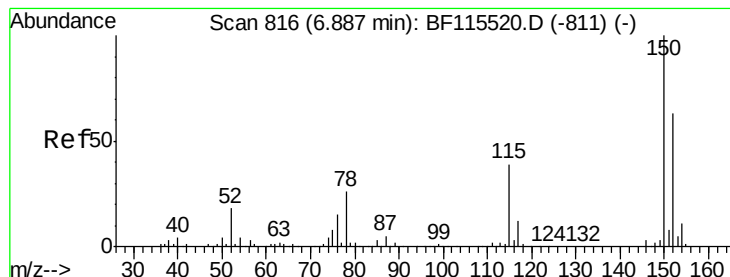


#1




1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 6.87 min Scan# 813
 Delta R.T. -0.01 min
 Lab File: BF115824.D
 Acq: 27 Jul 2019 12:16

Instrument :
 BNA_F
 ClientSampleId :
 55-ST-19

Tot Ion:152 Resp: 144179
 Ion Ratio Lower Upper
 152 100
 150 156.8 126.6 189.8
 115 63.8 47.8 71.6

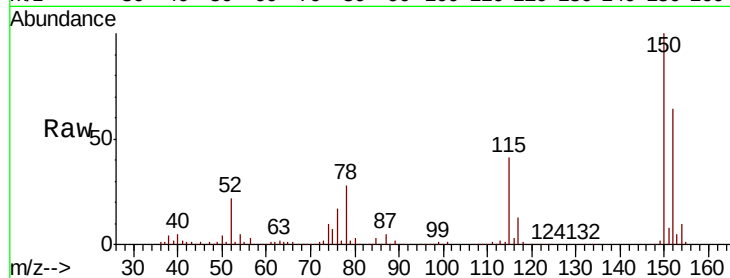


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

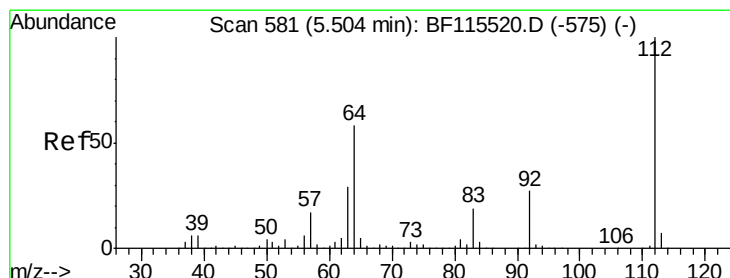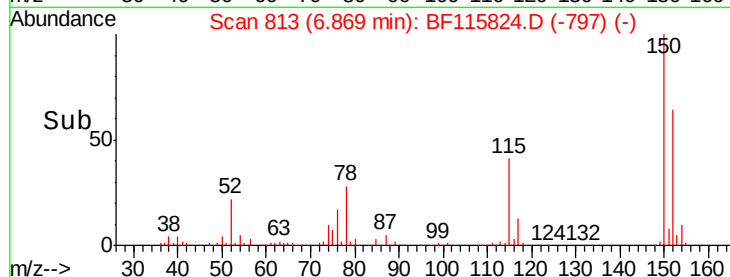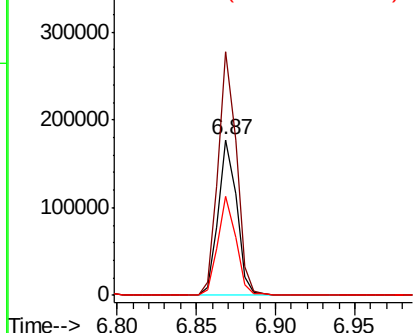



#5


2-Fluorophenol
 Concen: 40.990 ng
 RT: 5.49 min Scan# 579
 Delta R.T. -0.00 min
 Lab File: BF115824.D
 Acq: 27 Jul 2019 12:16

Tgt Ion:112 Resp: 361301
 Ion Ratio Lower Upper
 112 100
 64 55.9 45.8 68.8
 63 29.5 23.6 35.4

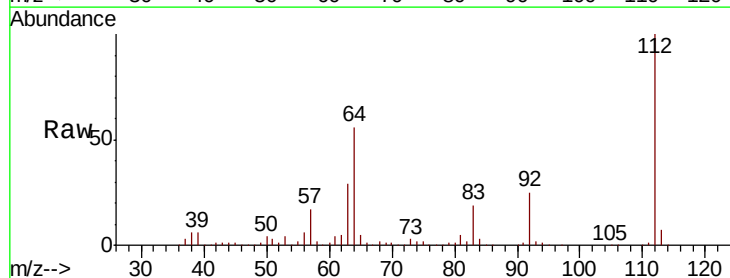

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BF1
 Ion 63.00 (62.70 to 63.70): BF1

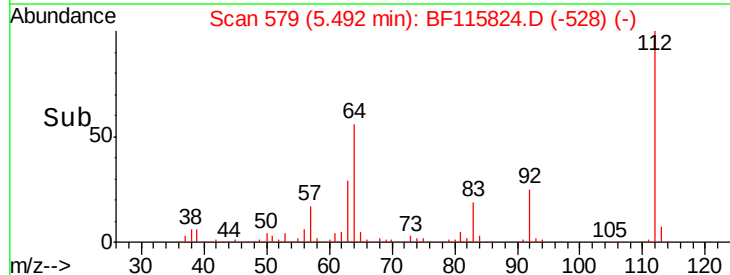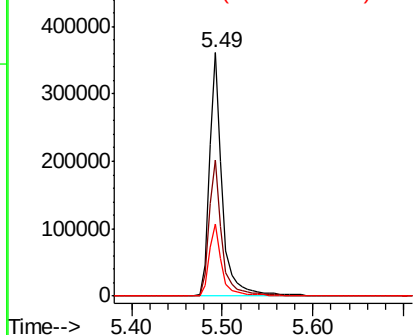

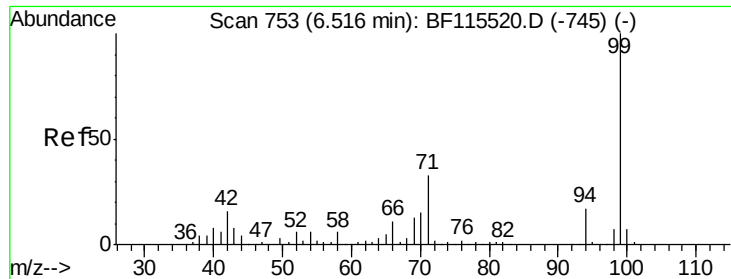

#7

Phenol-d6

Concen: 25.622 ng

RT: 6.49 min Scan# 749

Delta R.T. -0.01 min

Lab File: BF115824.D

Acq: 27 Jul 2019 12:16

Instrument :

BNA_F

ClientSampleId :

55-ST-19


Tot Ion: 99 Resp: 286568

Ion Ratio Lower Upper

99 100

42 18.6 13.4 20.2




71 33.2 26.7 40.1

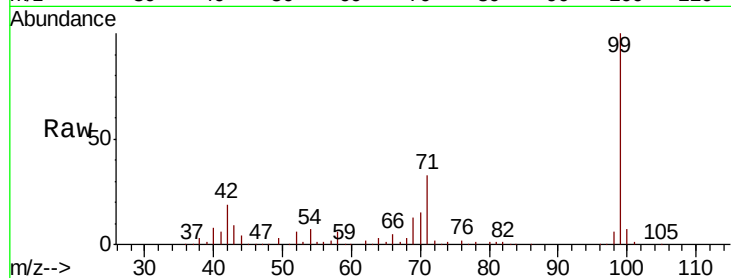

Abundance Ion 99.00 (98.70 to 99.70): BF1

Ion 42.00 (41.70 to 42.70): BF1

Ion 71.00 (70.70 to 71.70): BF1

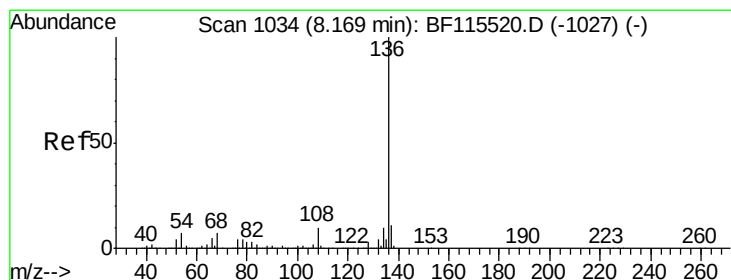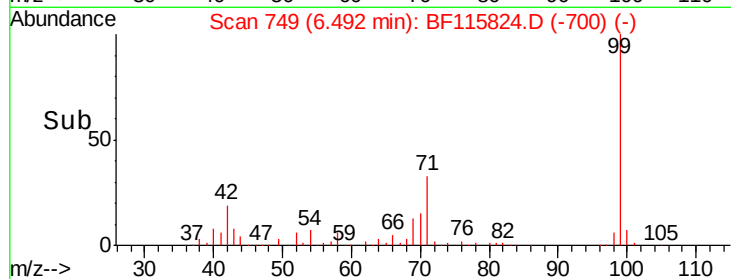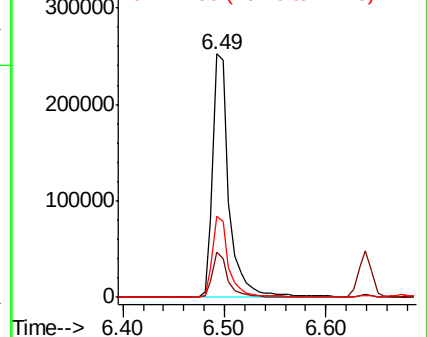

#21

Naphthalene-d8

Concen: 20.000 ng

RT: 8.15 min Scan# 1031

Delta R.T. -0.01 min

Lab File: BF115824.D

Acq: 27 Jul 2019 12:16

Tgt Ion: 136 Resp: 542067


Ion Ratio Lower Upper

136 100

137 10.8 8.7 13.1

54 7.1 5.0 7.6

68 6.4 4.7 7.1


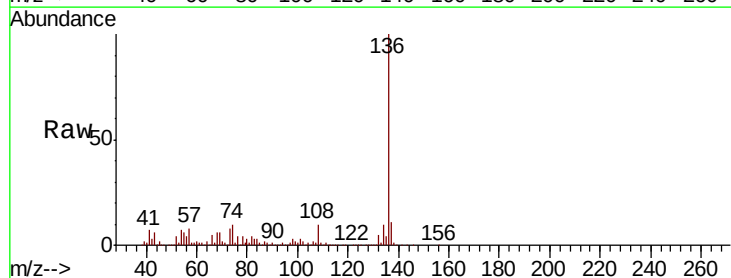



Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BF1

Ion 68.00 (67.70 to 68.70): BF1

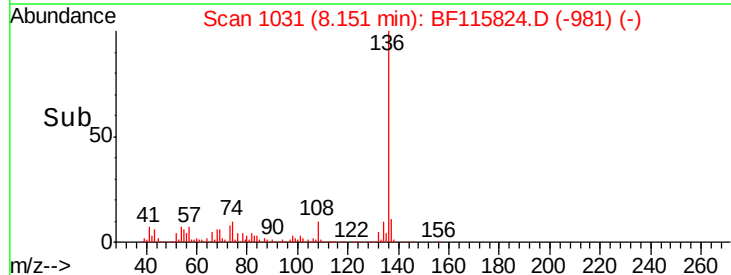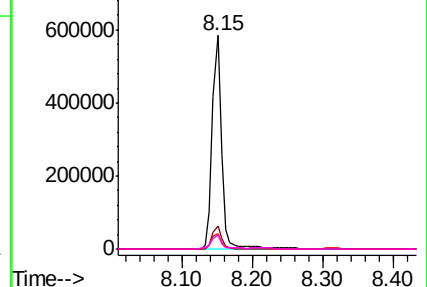


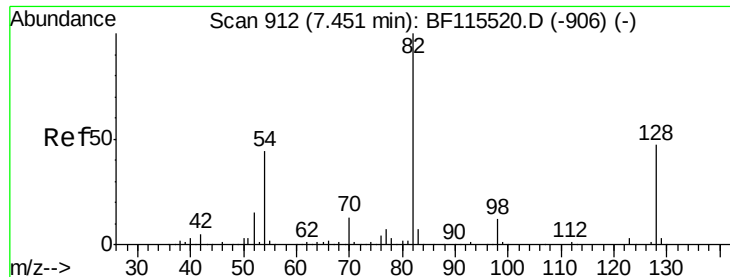




#23
 Nitrobenzene-d5
 Concen: 96.085 ng
 RT: 7.43 min Scan# 909
 Delta R.T. -0.00 min
 Lab File: BF115824.D
 Acq: 27 Jul 2019 12:16

Instrument :
 BNA_F
 ClientSampleId :
 55-ST-19

Tot Ion: 82 Resp: 895745
 Ion Ratio Lower Upper
 82 100
 128 48.3 36.6 55.0
 54 44.3 36.6 54.8

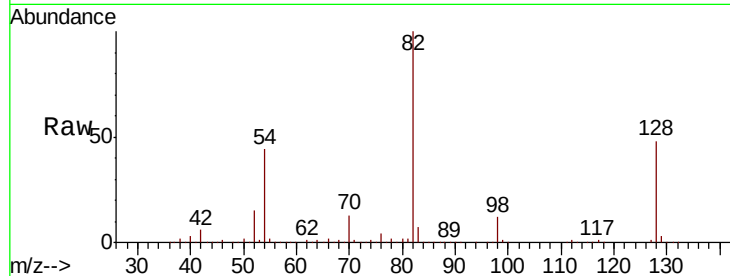


Abundance Ion 82.00 (81.70 to 82.70): BF1
 Ion 128.00 (127.70 to 128.70): E
 Ion 54.00 (53.70 to 54.70): BF1

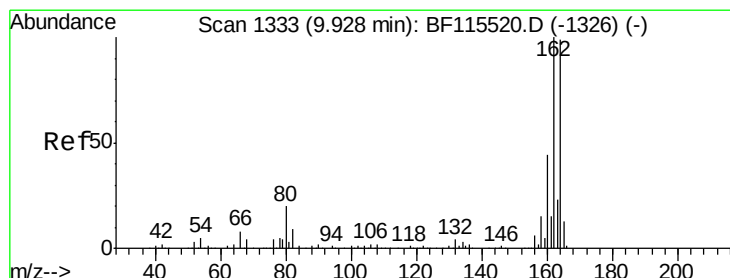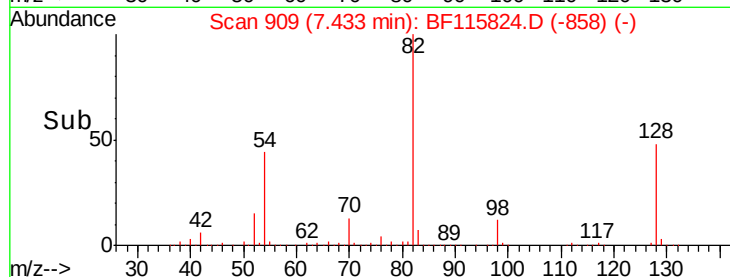
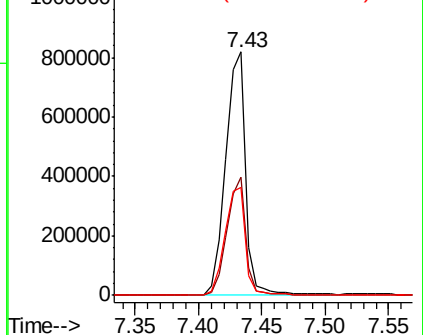



#39
 Acenaphthene-d10
 Concen: 20.000 ng
 RT: 9.90 min Scan# 1329
 Delta R.T. -0.01 min
 Lab File: BF115824.D
 Acq: 27 Jul 2019 12:16

Tgt Ion:164 Resp: 299967
 Ion Ratio Lower Upper
 164 100
 162 101.2 81.8 122.6
 160 45.7 37.5 56.3

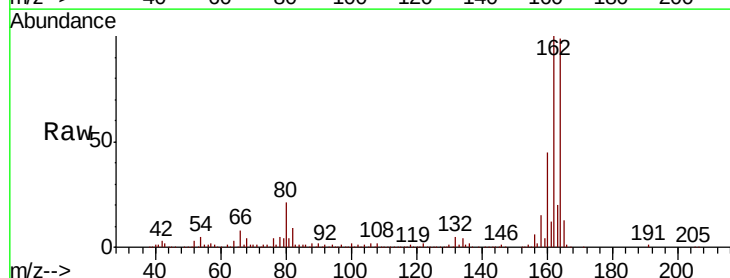

Abundance Ion 164.00 (163.70 to 164.70): E
 Ion 162.00 (161.70 to 162.70): E
 Ion 160.00 (159.70 to 160.70): E

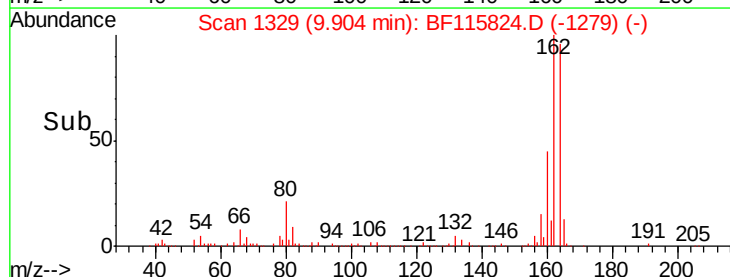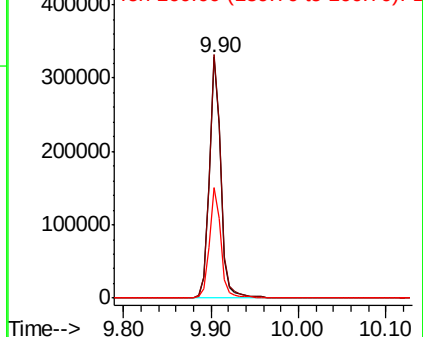


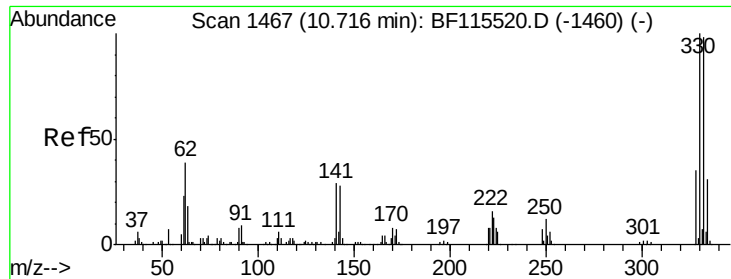

#42
 2,4,6-Tribromophenol
 Concen: 82.656 ng
 RT: 10.70 min Scan# 1464
 Delta R.T. -0.00 min
 Lab File: BF115824.D
 Acq: 27 Jul 2019 12:16

Instrument :
 BNA_F
 ClientSampleId :
 55-ST-19

Tot Ion	Ratio	Lower	Upper
330	100		
332	95.6	76.1	114.1
141	34.1	25.9	38.9



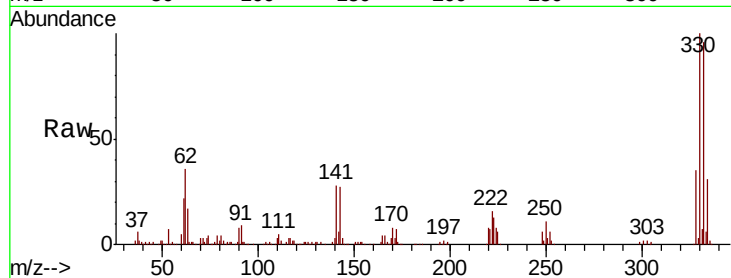


Abundance

Ion 329.80 (329.50 to 330.50): E


Ion 331.80 (331.50 to 332.50): E

Ion 141.00 (140.70 to 141.70): E

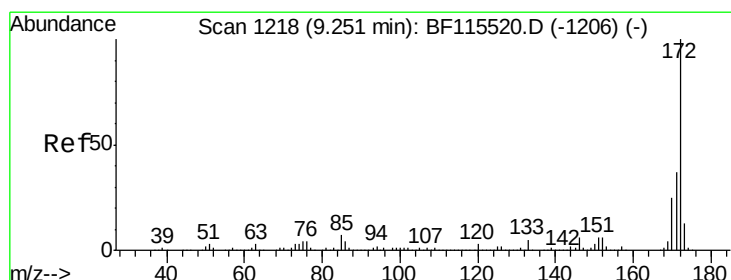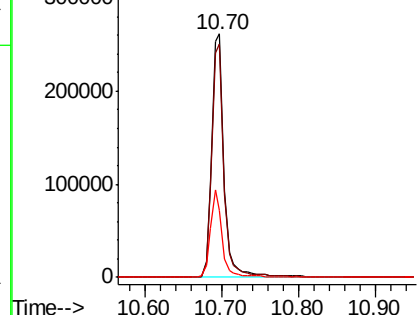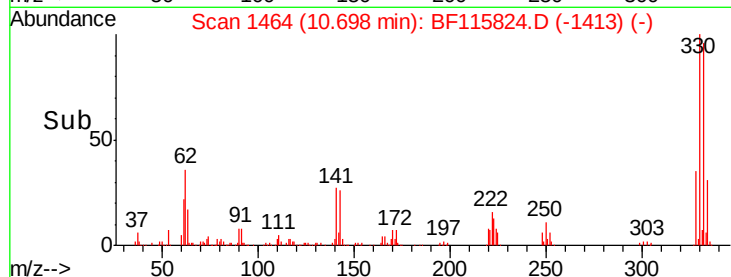

#45
 2-Fluorobiphenyl
 Concen: 93.378 ng
 RT: 9.23 min Scan# 1214
 Delta R.T. -0.01 min
 Lab File: BF115824.D
 Acq: 27 Jul 2019 12:16

Tgt Ion	Ratio	Lower	Upper
172	100		
171	36.5	29.0	43.4
170	25.1	20.1	30.1


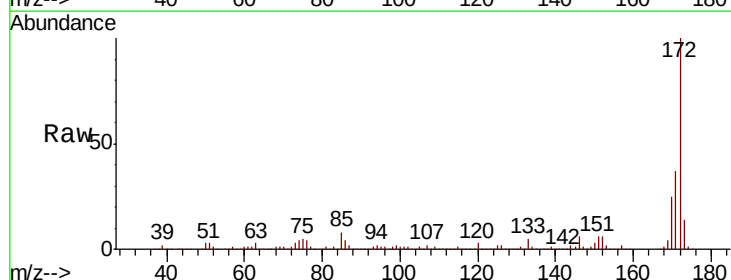



Abundance

Ion 172.00 (171.70 to 172.70): E

Ion 171.00 (170.70 to 171.70): E

Ion 170.00 (169.70 to 170.70): E

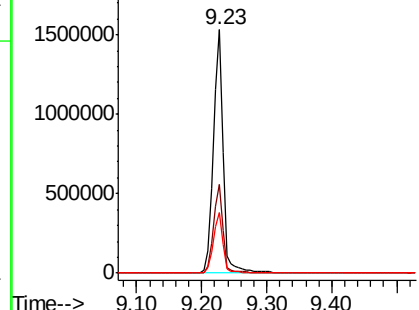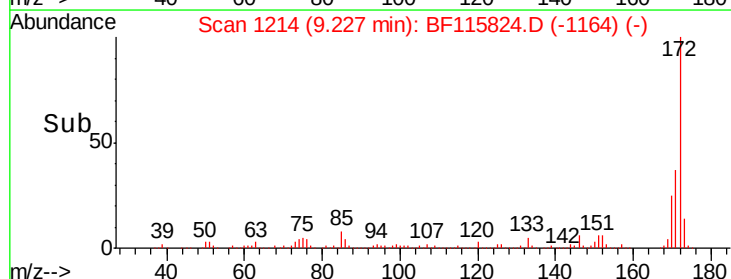

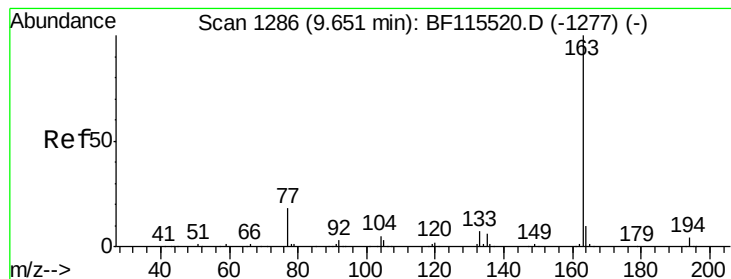

#50

Dimethylphthalate

Concen: 5.998 ng

RT: 9.62 min Scan# 1280

Delta R.T. -0.02 min

Lab File: BF115824.D

Acq: 27 Jul 2019 12:16

Instrument :

BNA_F

ClientSampleId :

55-ST-19


Tot Ion:163 Resp: 135374

Ion Ratio Lower Upper




163 100

194 4.1 3.2 4.8

164 10.0 8.3 12.5

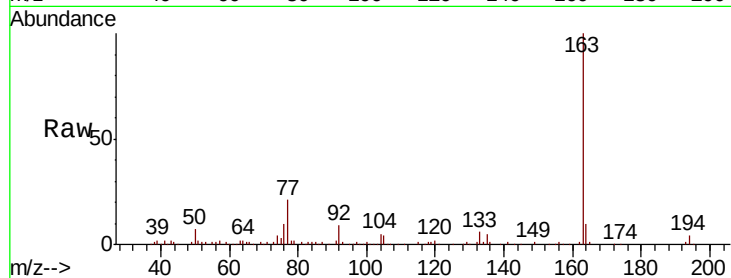

Abundance Ion 163.00 (162.70 to 163.70): E
Ion 194.00 (193.70 to 194.70): E
Ion 164.00 (163.70 to 164.70): E

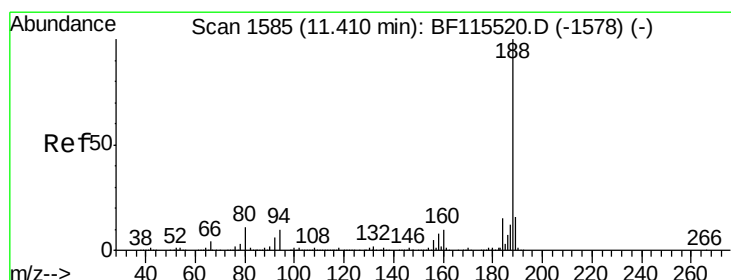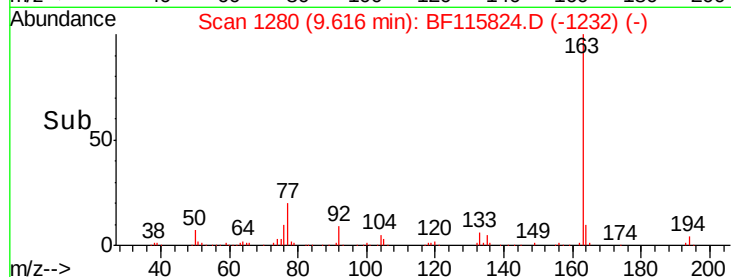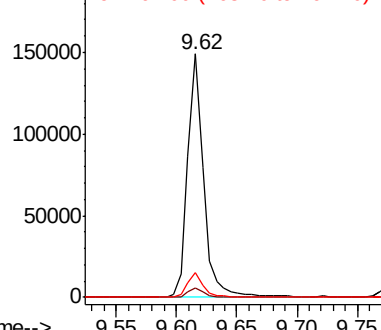

#64

Phenanthrene-d10

Concen: 20.000 ng

RT: 11.39 min Scan# 1582

Delta R.T. -0.00 min

Lab File: BF115824.D

Acq: 27 Jul 2019 12:16


Tgt Ion:188 Resp: 523240

Ion Ratio Lower Upper



188 100


94 8.9 8.2 12.2

80 9.8 9.0 13.6

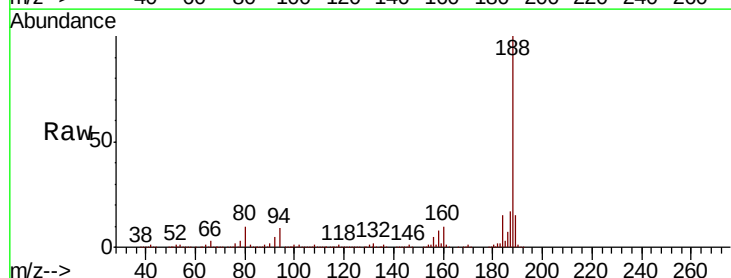

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BF1
Ion 80.00 (79.70 to 80.70): BF1



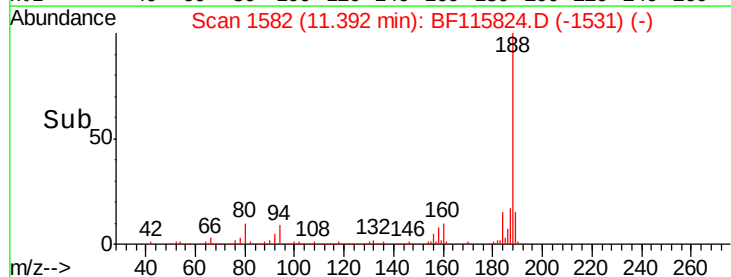
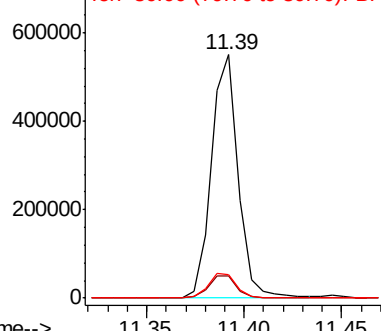


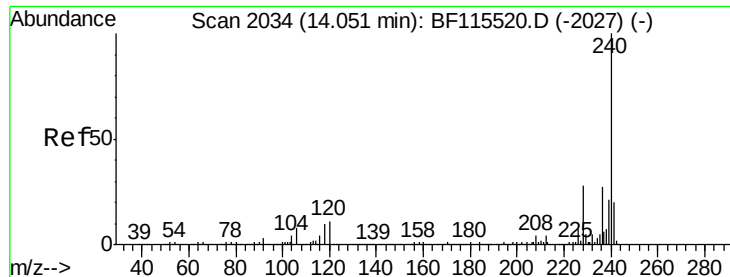

#76
Chrysene-d12
Concen: 20.000 ng
RT: 14.03 min Scan# 2030
Delta R.T. -0.01 min
Lab File: BF115824.D
Acq: 27 Jul 2019 12:16




Instrument :
BNA_F
ClientSampleId :
55-ST-19


Tot Ion:240 Resp: 375472
Ion Ratio Lower Upper
240 100
120 11.8 10.0 15.0
236 27.1 21.8 32.6

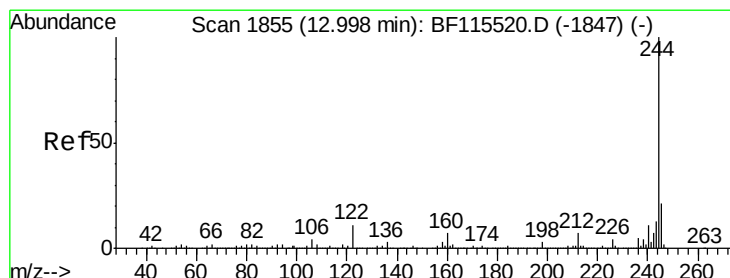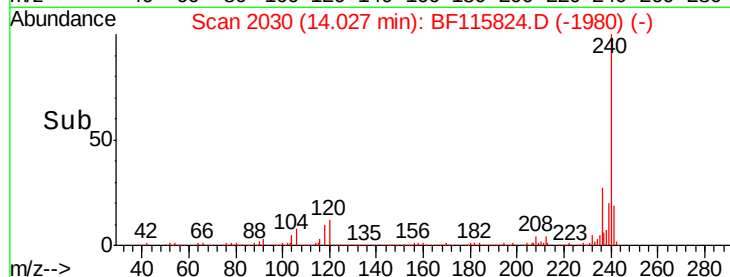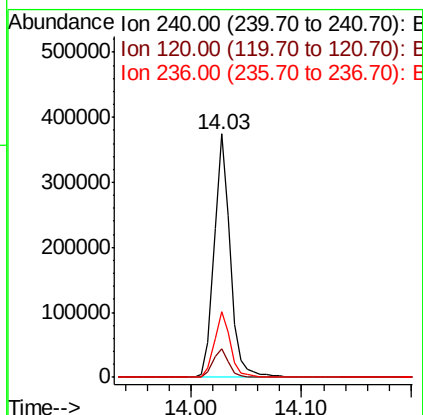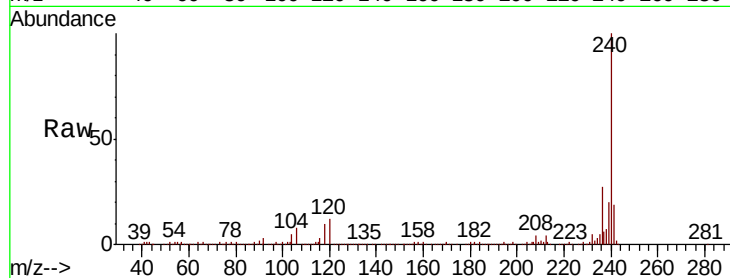

#79
Terphenyl-d14
Concen: 81.486 ng
RT: 12.97 min Scan# 1851
Delta R.T. -0.01 min
Lab File: BF115824.D
Acq: 27 Jul 2019 12:16

Tgt Ion:244 Resp: 1658160
Ion Ratio Lower Upper
244 100
212 7.2 5.5 8.3
122 12.0 8.2 12.4

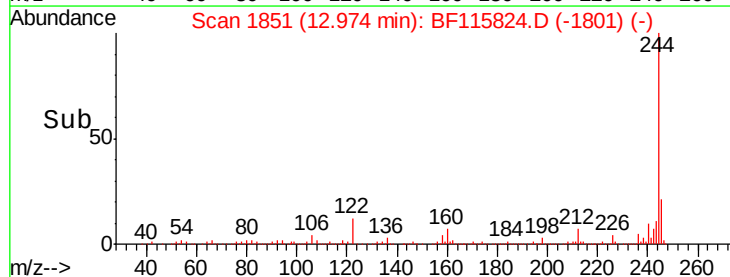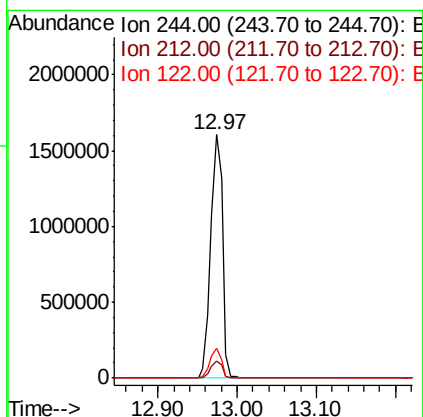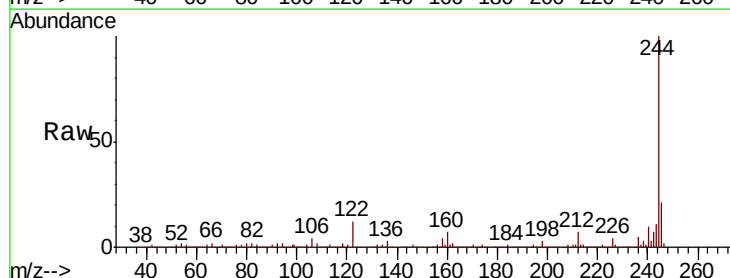

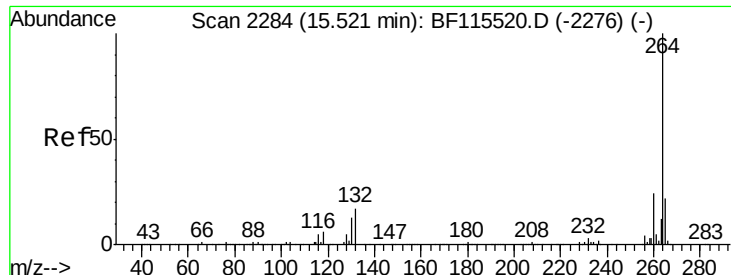

#87
Pervlene-d12
Concen: 20.000 ng
RT: 15.50 min Scan# 2280
Delta R.T. -0.00 min
Lab File: BF115824.D
Acq: 27 Jul 2019 12:16

Instrument :
BNA_F
ClientSampleId :
55-ST-19

Tot Ion	Ratio	Lower	Upper
264	100		
260	24.4	19.8	29.6
265	21.2	17.5	26.3

