


Data Path : Z:\SVOASRV\HPCHEM1\BNA_F\DATA\BF072719\
 Data File : BF115815.D
 Acq On : 27 Jul 2019 7:43
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF071219.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 29 16:38:26 2019

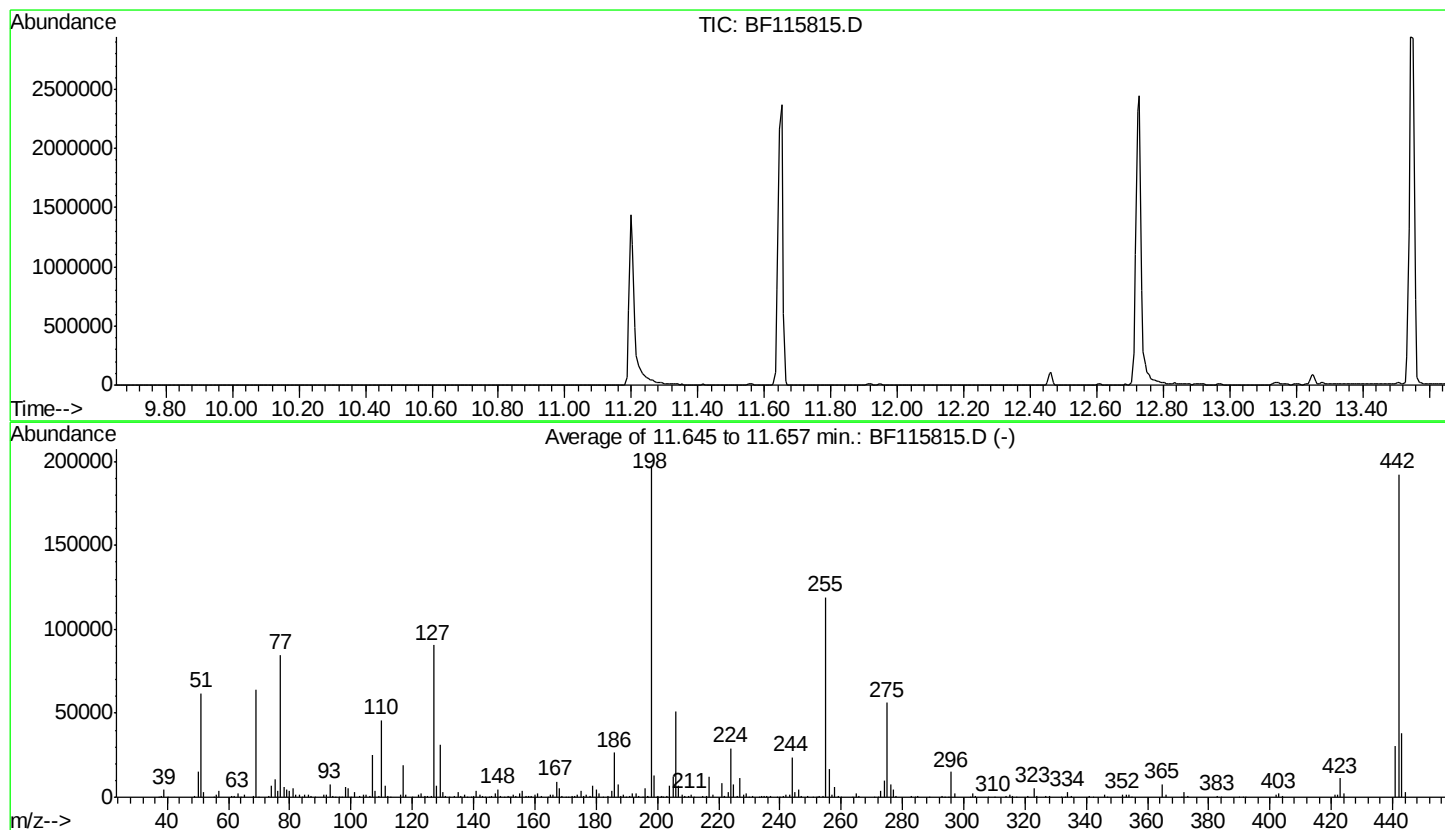

AutoFind: Scans 1625, 1626, 1627; Background Corrected with Scan 1619

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	31.4	62137	PASS
68	69	0.00	2	1.4	928	PASS
69	198	0.00	100	32.4	64072	PASS
70	69	0.00	2	0.5	343	PASS
127	198	10	80	45.9	90645	PASS
197	198	0.00	2	0.3	513	PASS
198	198	100	100	100.0	197605	PASS
199	198	5	9	6.7	13297	PASS
275	198	10	60	28.5	56402	PASS
365	198	1	100	3.9	7747	PASS
441	198	0.01	100	15.6	30754	PASS
442	198	50	100	97.4	192405	PASS
443	442	15	24	19.9	38218	PASS