
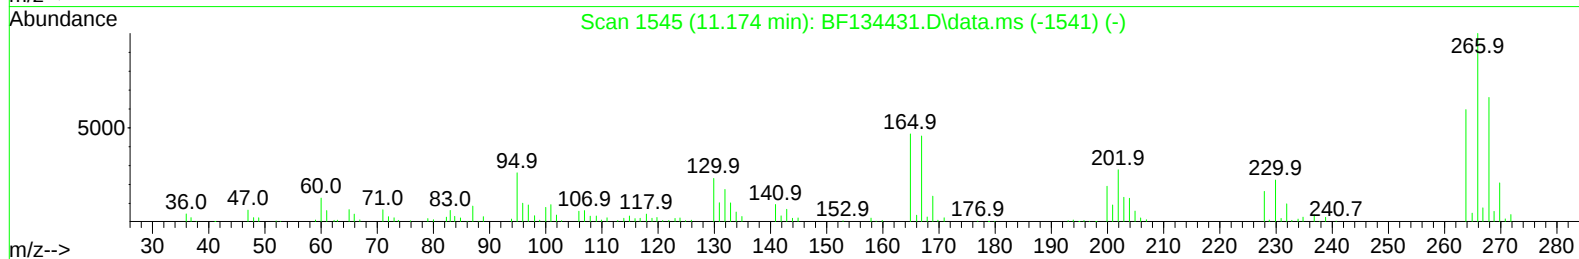
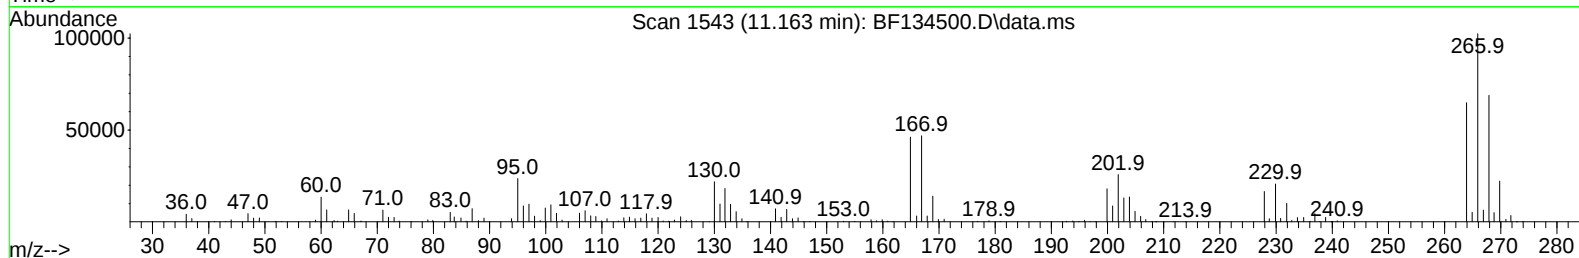


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072723\
Data File : BF134500.D
Acq On : 27 Jul 2023 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 12:13:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

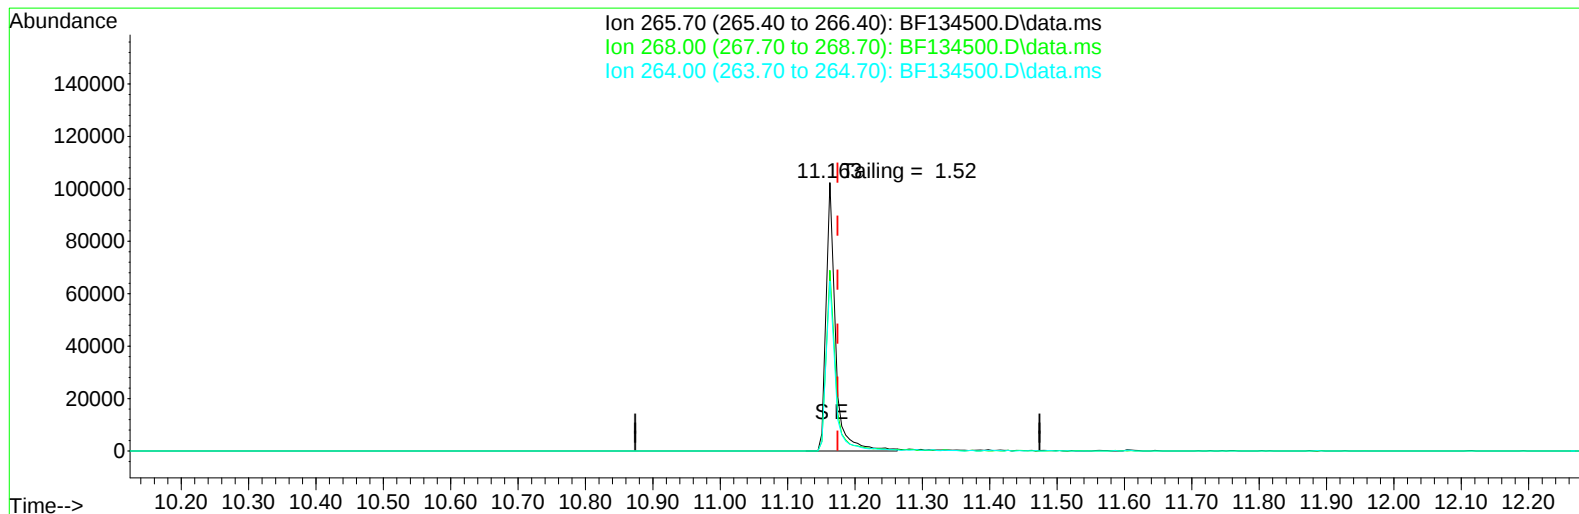

TIC: BF134500.D\data.ms

(70) Pentachlorophenol (C)




11.163min (-0.011) 29701.02 ng

response 100422

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.32
264.00	59.70	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072723\
Data File : BF134500.D
Acq On : 27 Jul 2023 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 27 12:13:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

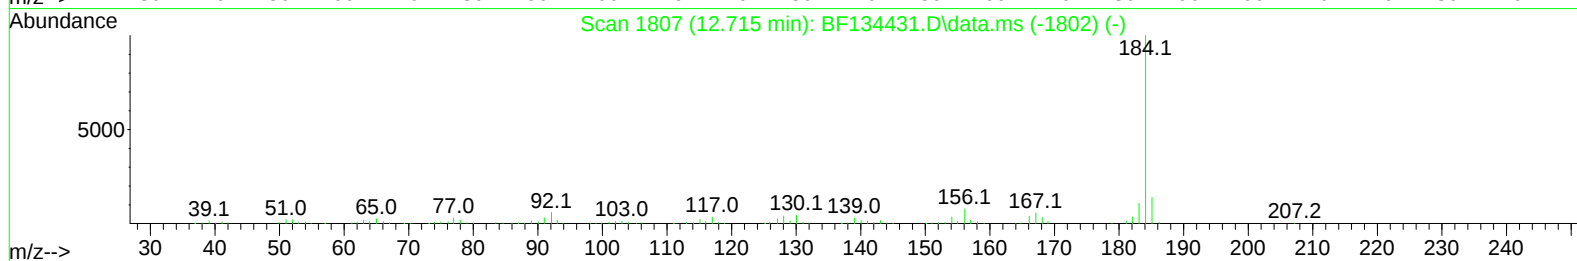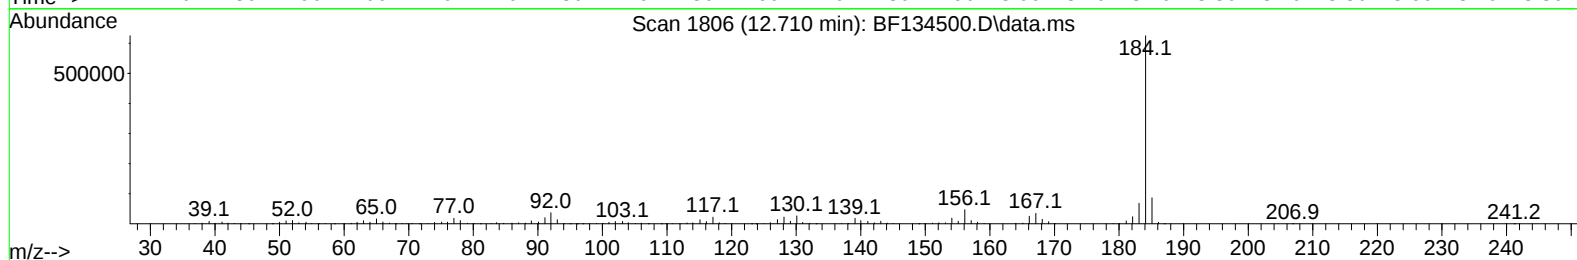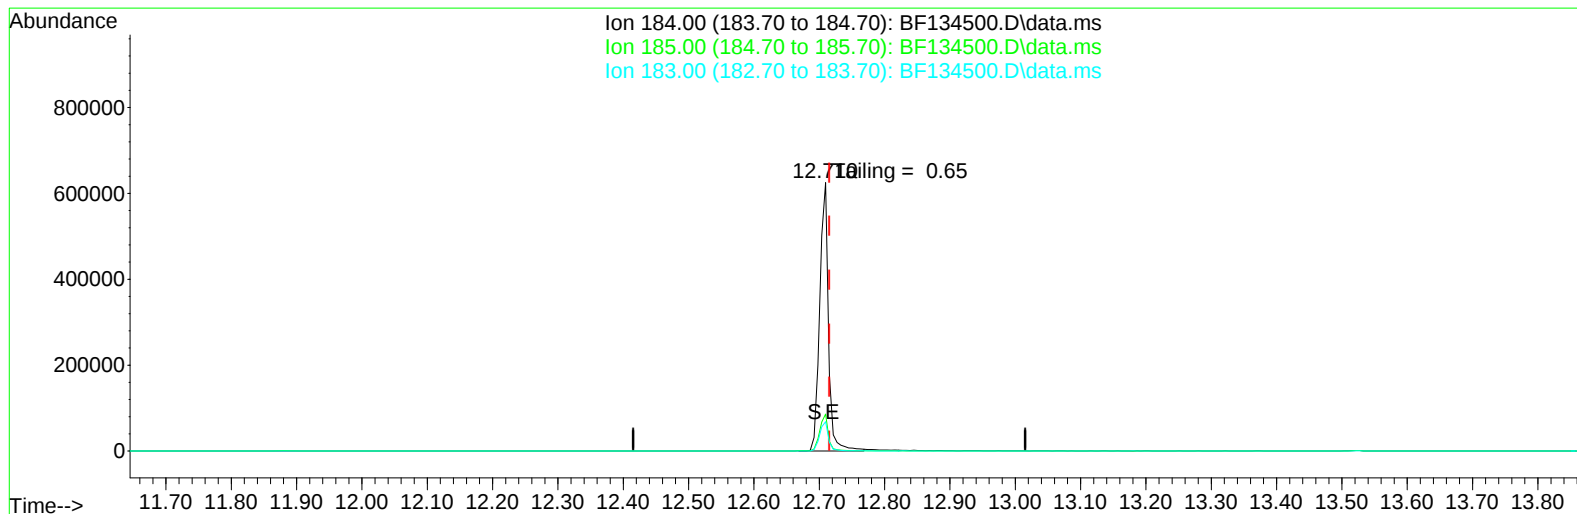

TIC: BF134500.D\data.ms

(77) Benzidine

12.710min (-0.005) 463426.84 ng

response 593706

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.78
183.00	10.80	10.93
0.00	0.00	0.00