
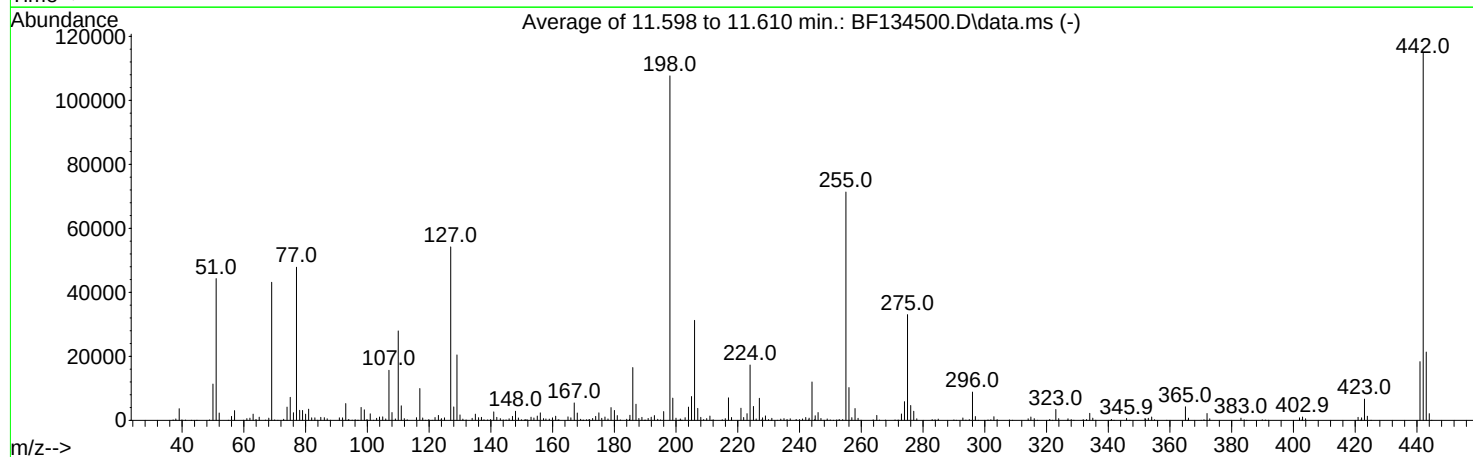


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072723\
Data File : BF134500.D
Acq On : 27 Jul 2023 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\BFDDTBREAKDOWN-8270.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Sep 01 16:14:27 2010

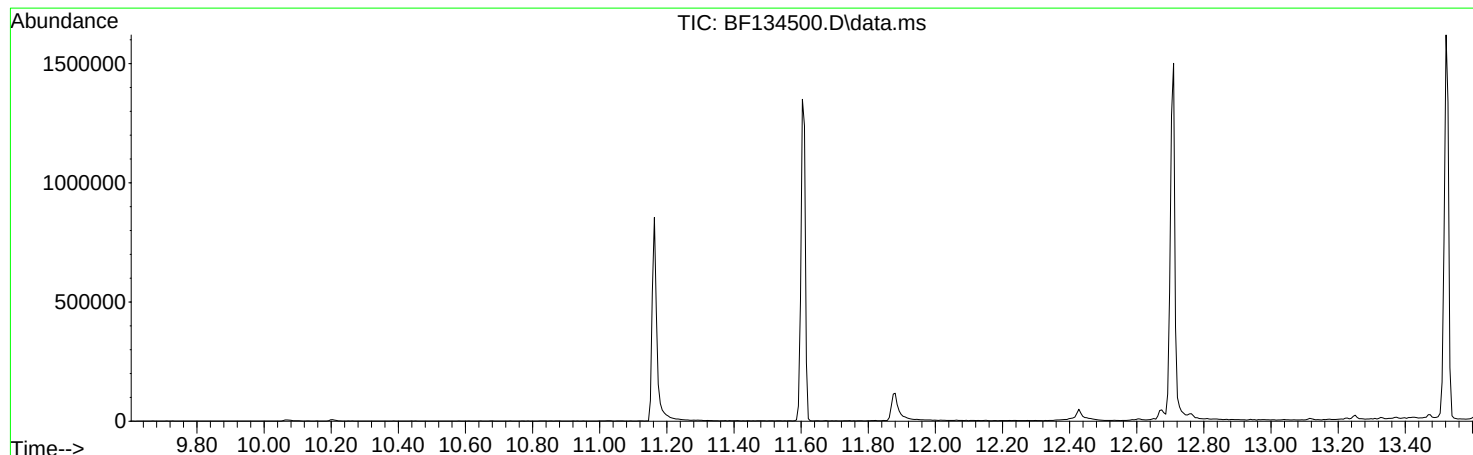




AutoFind: Scans 1617, 1618, 1619; Background Corrected with Scan 1612

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.1	44291	PASS
68	69	0.00	2	1.6	692	PASS
69	198	0.00	100	40.1	43176	PASS
70	69	0.00	2	0.4	170	PASS
127	198	10	80	50.3	54189	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	107683	PASS
199	198	5	9	6.5	6952	PASS
275	198	10	60	30.7	33071	PASS
365	198	1	100	3.9	4233	PASS
441	442	0.01	24	16.0	18339	PASS
442	198	50	100	106.8	114965	FAIL*
443	442	15	24	18.6	21353	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072723\
Data File : BF134500.D
Acq On : 27 Jul 2023 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 27 12:13:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

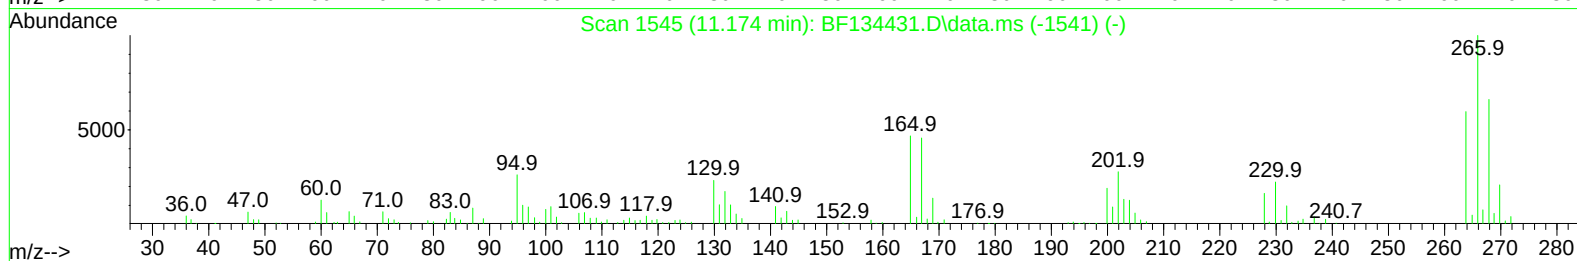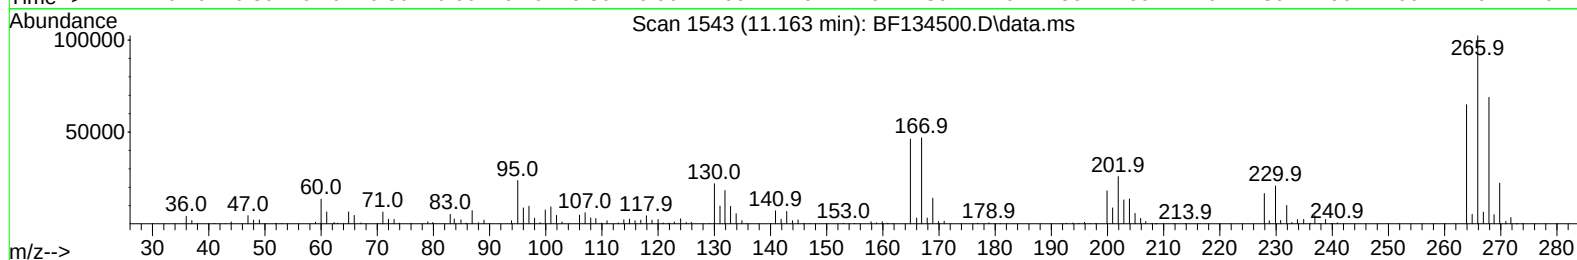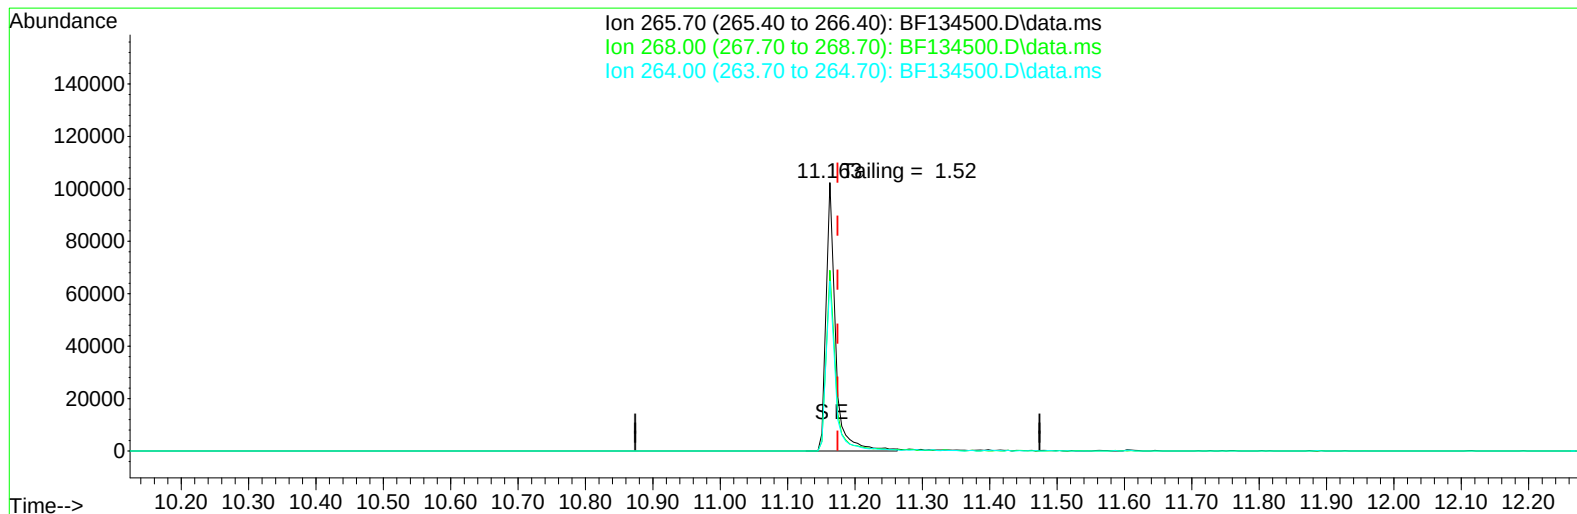

TIC: BF134500.D\data.ms

(70) Pentachlorophenol (C)

11.163min (-0.011) 29701.02 ng




response 100422

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	67.32
264.00	59.70	63.35
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072723\
Data File : BF134500.D
Acq On : 27 Jul 2023 09:35
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 27 12:13:09 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 25 01:46:04 2023
Response via : Initial Calibration

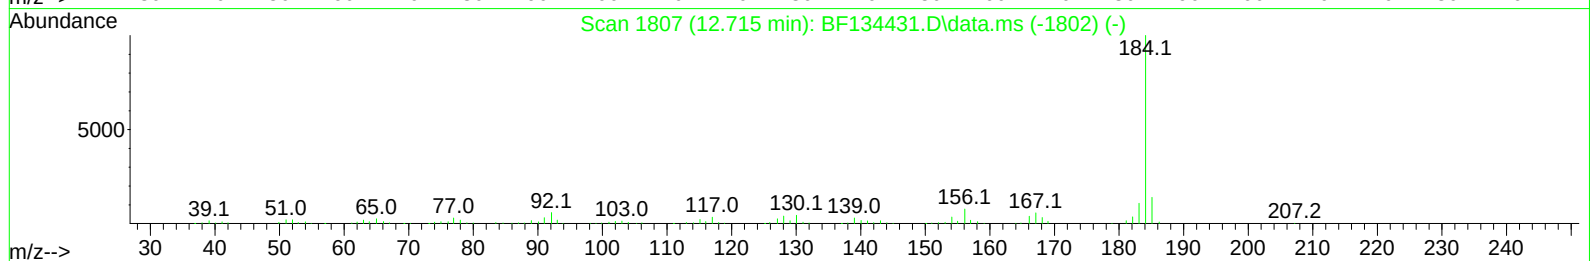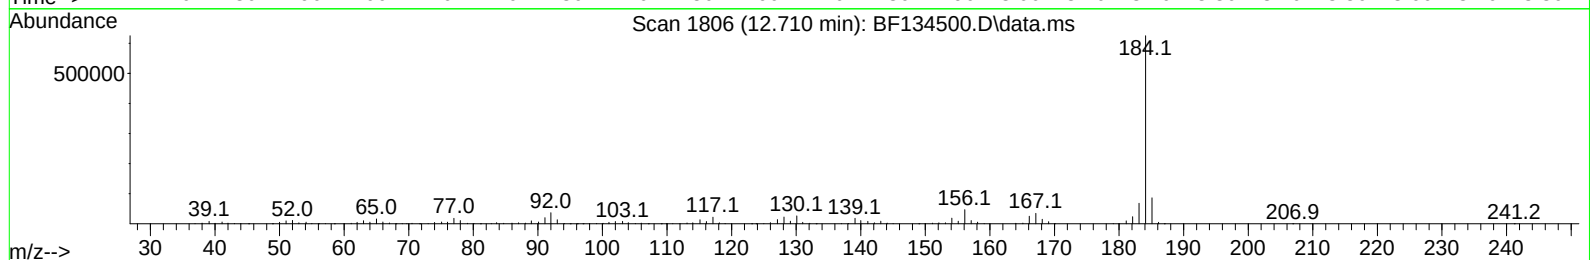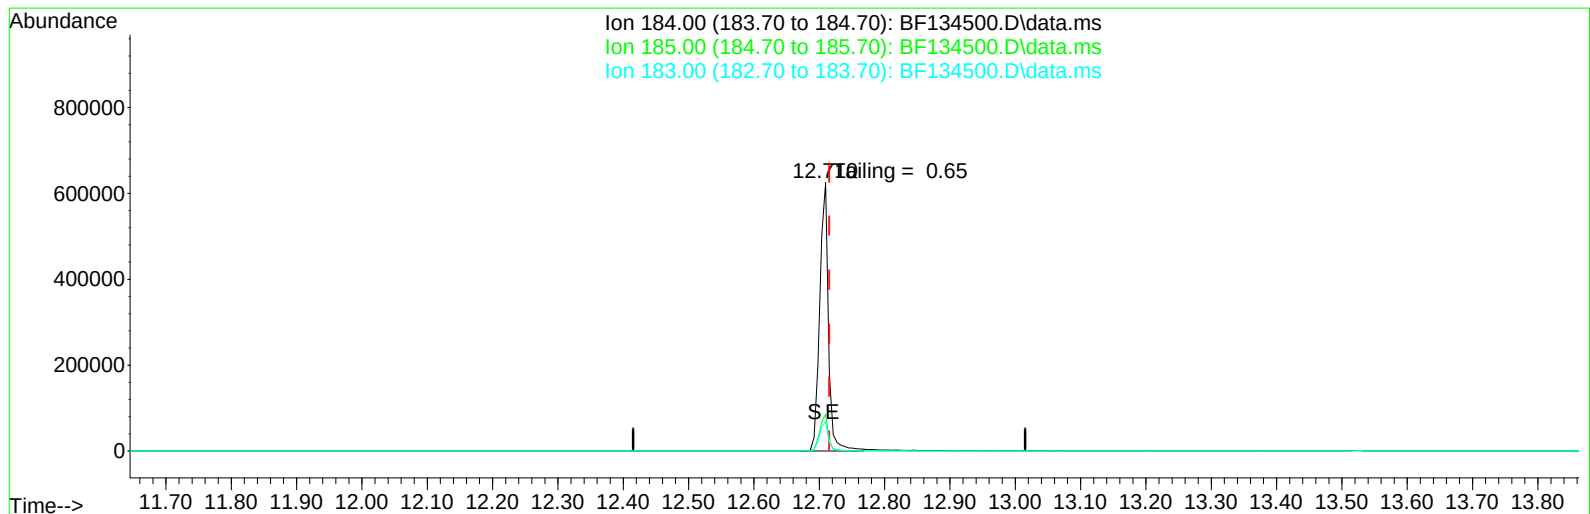

TIC: BF134500.D\data.ms

(77) Benzidine

12.710min (-0.005) 463426.84 ng

response 593706

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.78
183.00	10.80	10.93
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
7/27/2023	BNA_F	<u>BF134500.D</u>
Compound Name	Response	Retention Time
DDT	281727	13.521
DDD	3996	13.251
DDE	84	12.88
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4080	285807	1.43

Instrument :
BNA_F
ClientSampleId :
DFTPP