
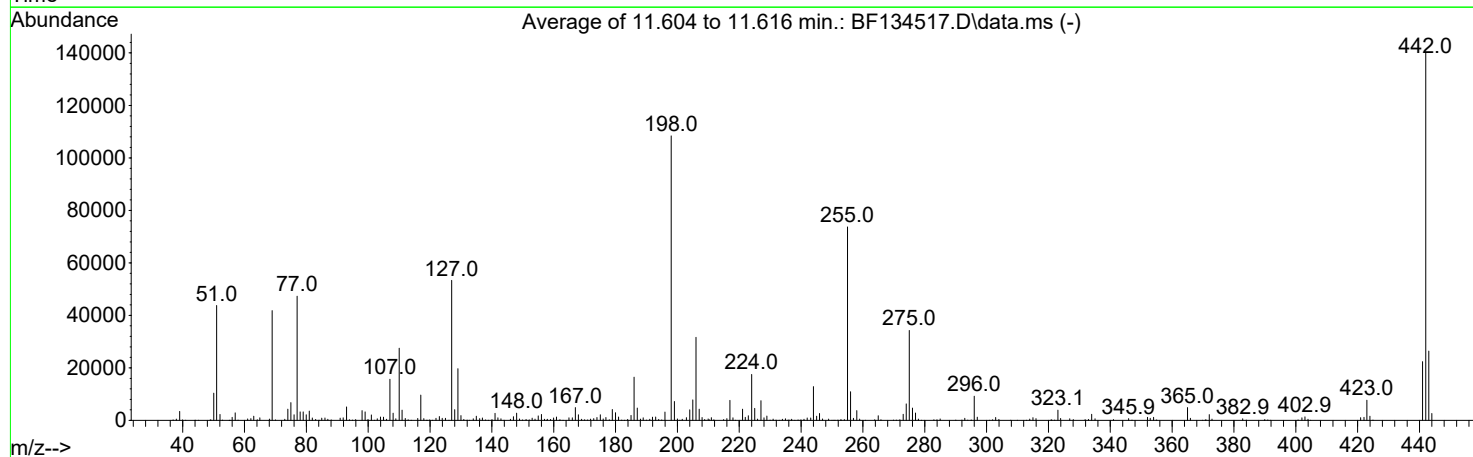


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072823\
Data File : BF134517.D
Acq On : 28 Jul 2023 15:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Jul 27 12:16:03 2023

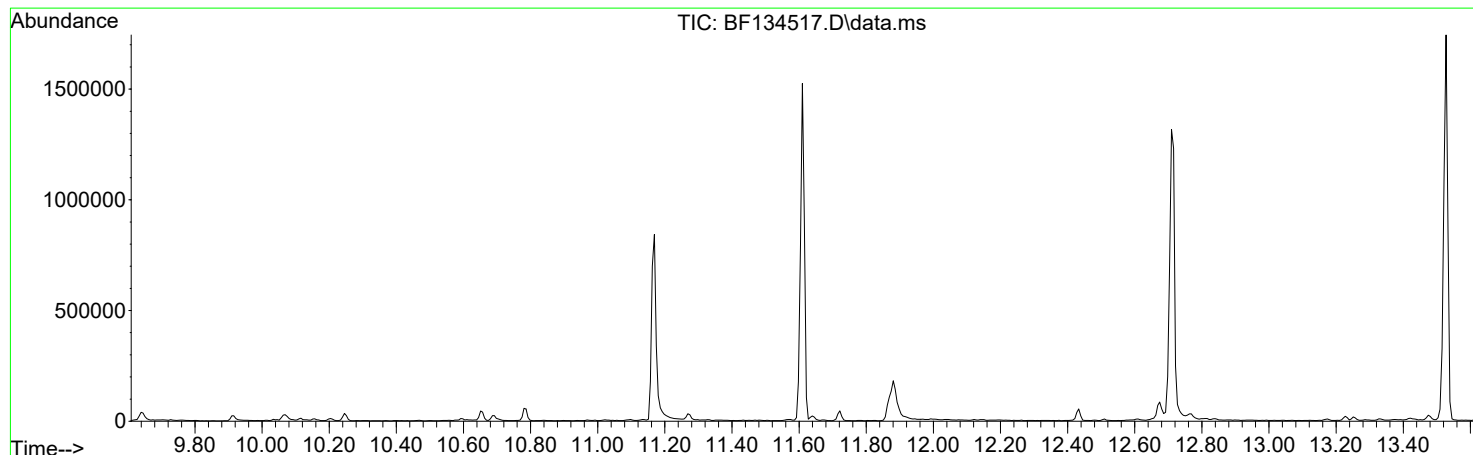

AutoFind: Scans 1618, 1619, 1620; Background Corrected with Scan 1613

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	40.4	43795	PASS
68	69	0.00	2	1.1	472	PASS
69	198	0.00	100	38.6	41834	PASS
70	69	0.00	2	0.5	193	PASS
127	198	10	80	49.2	53339	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	108419	PASS
199	198	5	9	6.6	7185	PASS
275	198	10	60	31.6	34291	PASS
365	198	1	100	4.5	4895	PASS
441	198	0.01	100	20.7	22396	PASS
442	442	50	100	100.0	140157	PASS
443	442	15	24	18.8	26379	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/28/2023	BNA_F	<u>BF134517.D</u>
Compound Name	Response	Retention Time
DDT	286144	13.527
DDD	6395	13.227
DDE	53	12.886
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6448	292592	2.20

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072823\
Data File : BF134517.D
Acq On : 28 Jul 2023 15:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 29 05:29:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 27 12:16:03 2023
Response via : Initial Calibration

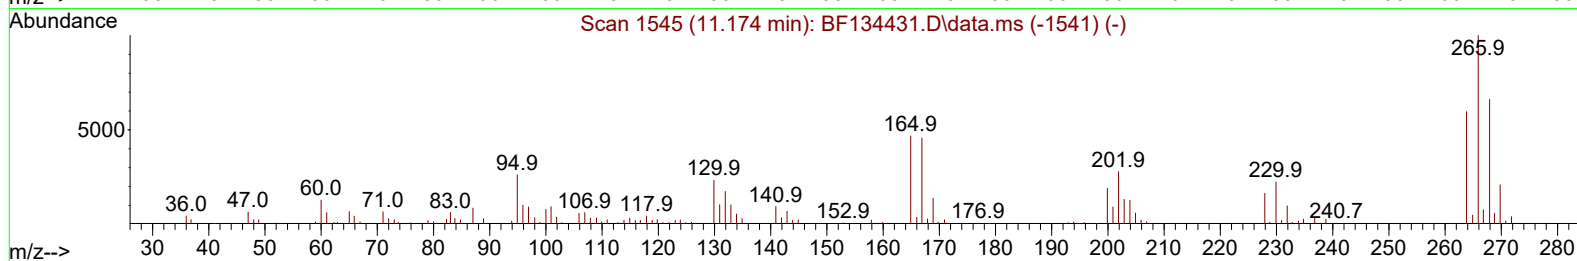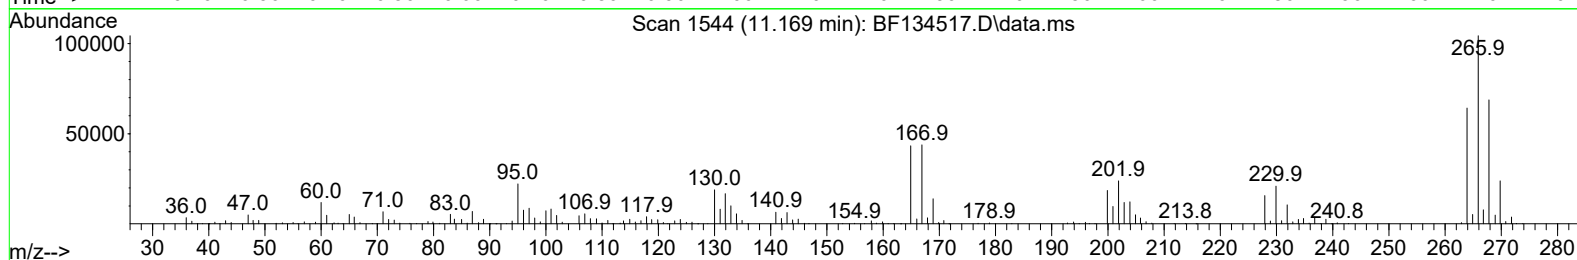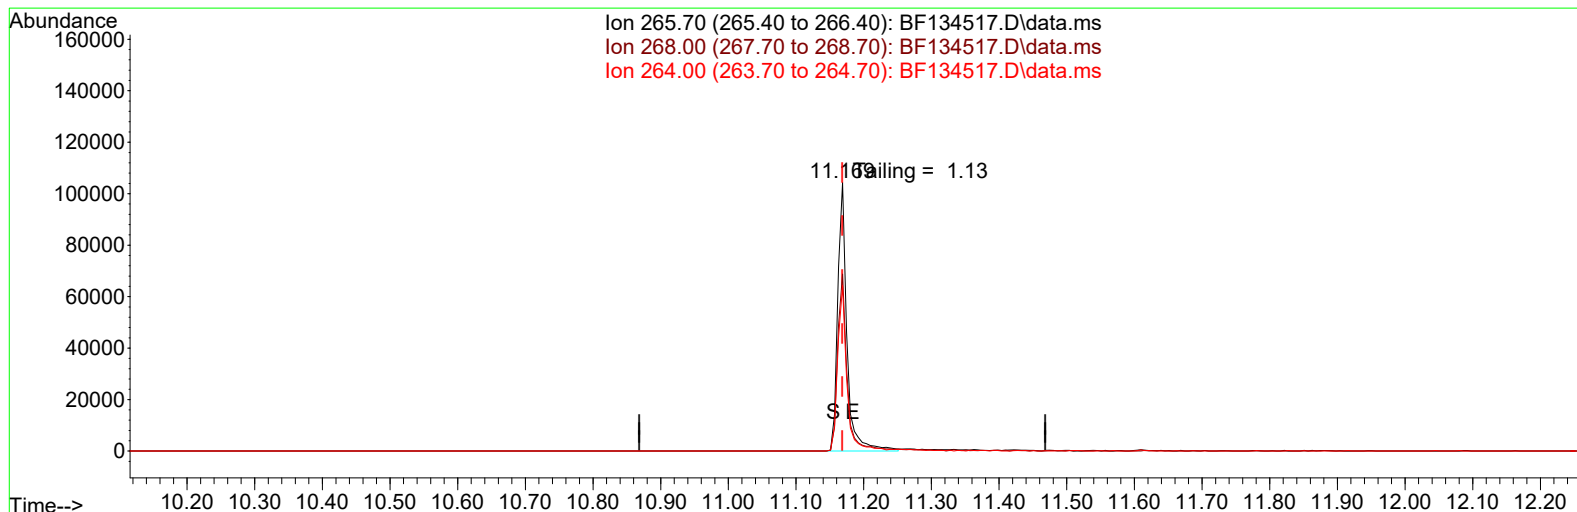

TIC: BF134517.D\data.ms

(70) Pentachlorophenol (C)

11.169min (+ 0.000) 38107.55 ng




response 99643

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	66.10	65.97
264.00	59.70	61.59
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072823\
Data File : BF134517.D
Acq On : 28 Jul 2023 15:21
Operator : CG\JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 29 05:29:18 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF072423.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Jul 27 12:16:03 2023
Response via : Initial Calibration

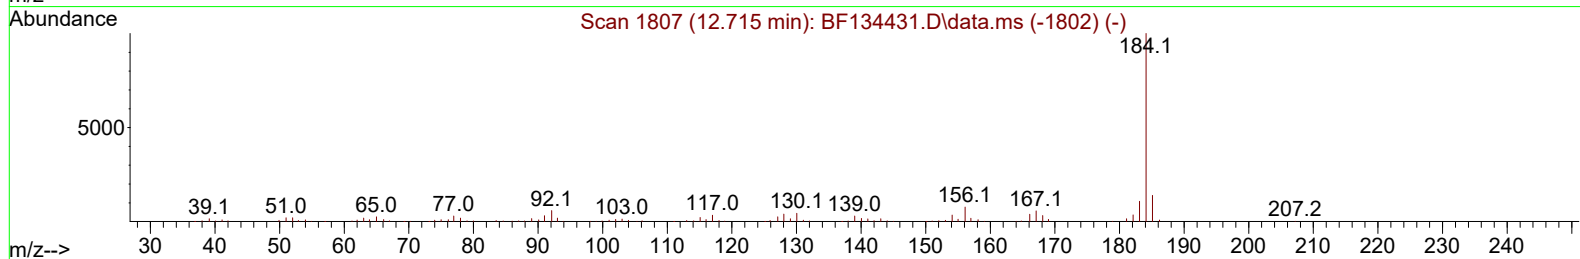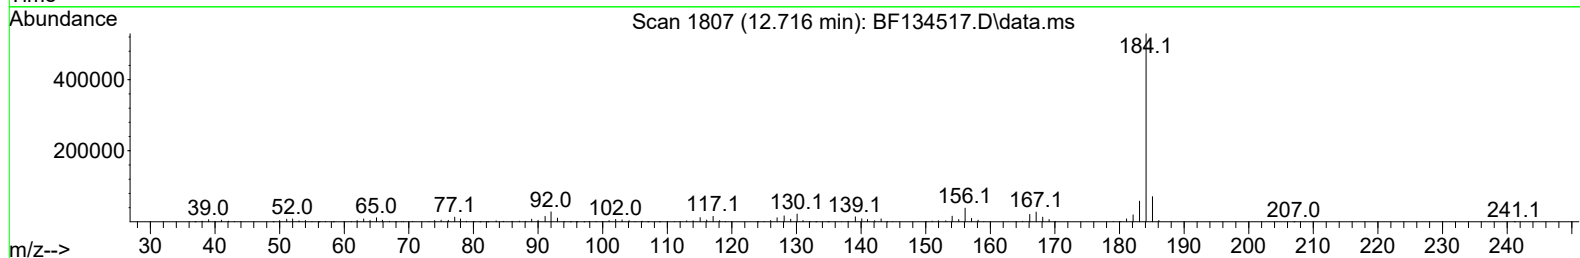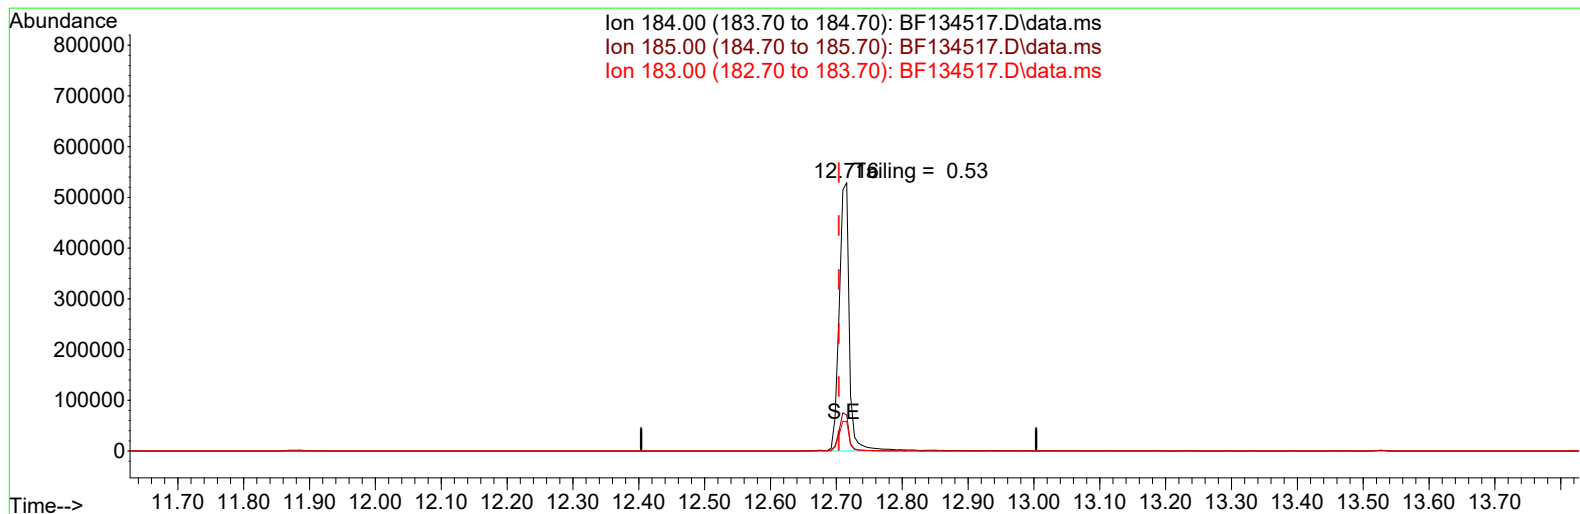

TIC: BF134517.D\data.ms

(77) Benzidine

12.716min (+ 0.012) 0.00 ng

response 563543

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.00	13.39
183.00	10.80	10.98
0.00	0.00	0.00