


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072924\
Data File : BF138667.D
Acq On : 29 Jul 2024 12:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Tue Jul 09 16:58:40 2024

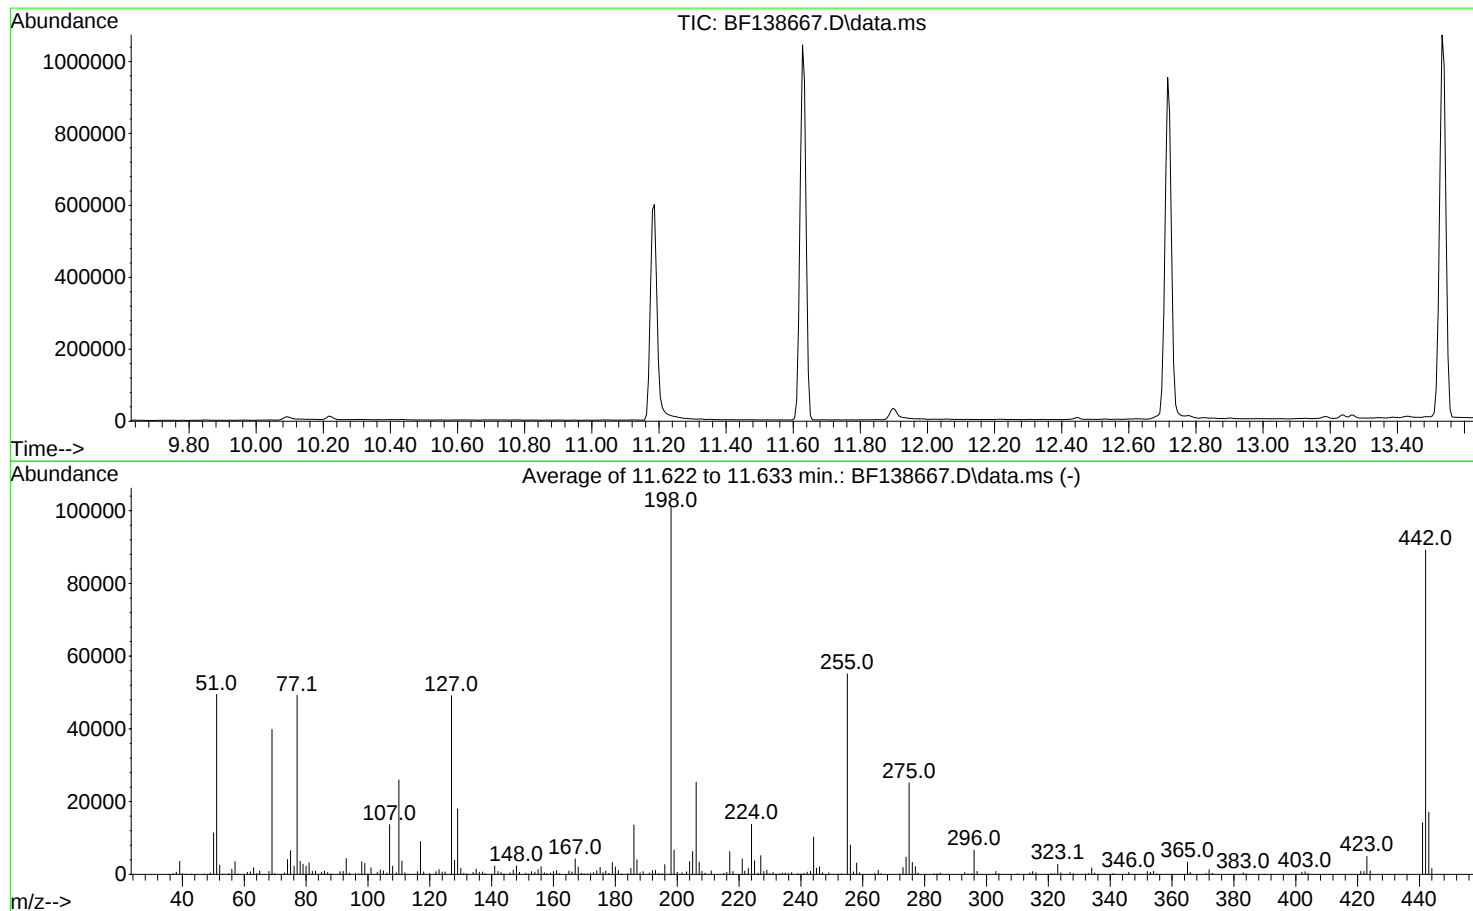

AutoFind: Scans 1620, 1621, 1622; Background Corrected with Scan 1614

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	48.9	49487	PASS
68	69	0.00	2	2.0	796	PASS
69	198	0.00	100	39.3	39803	PASS
70	69	0.00	2	0.6	242	PASS
127	198	10	80	48.5	49088	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	101157	PASS
199	198	5	9	6.6	6683	PASS
275	198	10	60	24.9	25171	PASS
365	198	1	100	3.3	3365	PASS
441	198	0.01	100	14.1	14233	PASS
442	442	50	100	100.0	89211	PASS
443	442	15	24	19.2	17122	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
7/29/2024	BNA_F	<u>BF138667.D</u>
Compound Name	Response	Retention Time
DDT	258888	13.533
DDD	6222	13.239
DDE	606	12.904
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
6828	265716	2.57

Instrument :
BNA_F
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072924\
Data File : BF138667.D
Acq On : 29 Jul 2024 12:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 29 13:32:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

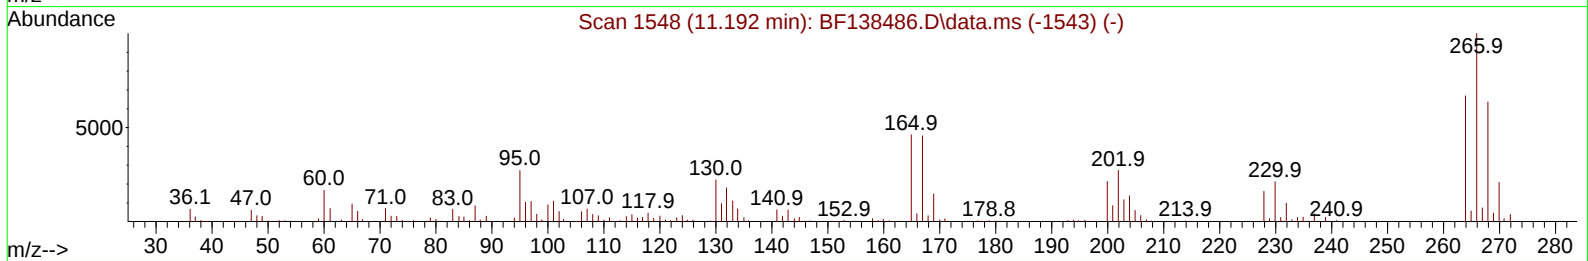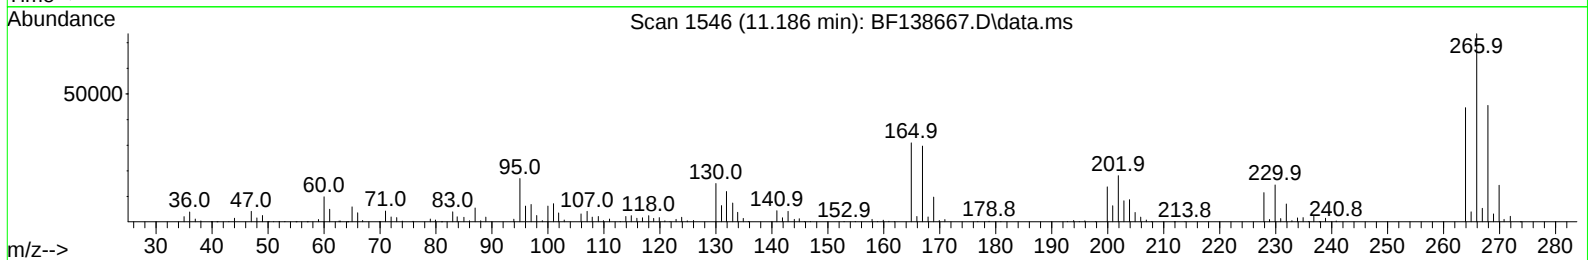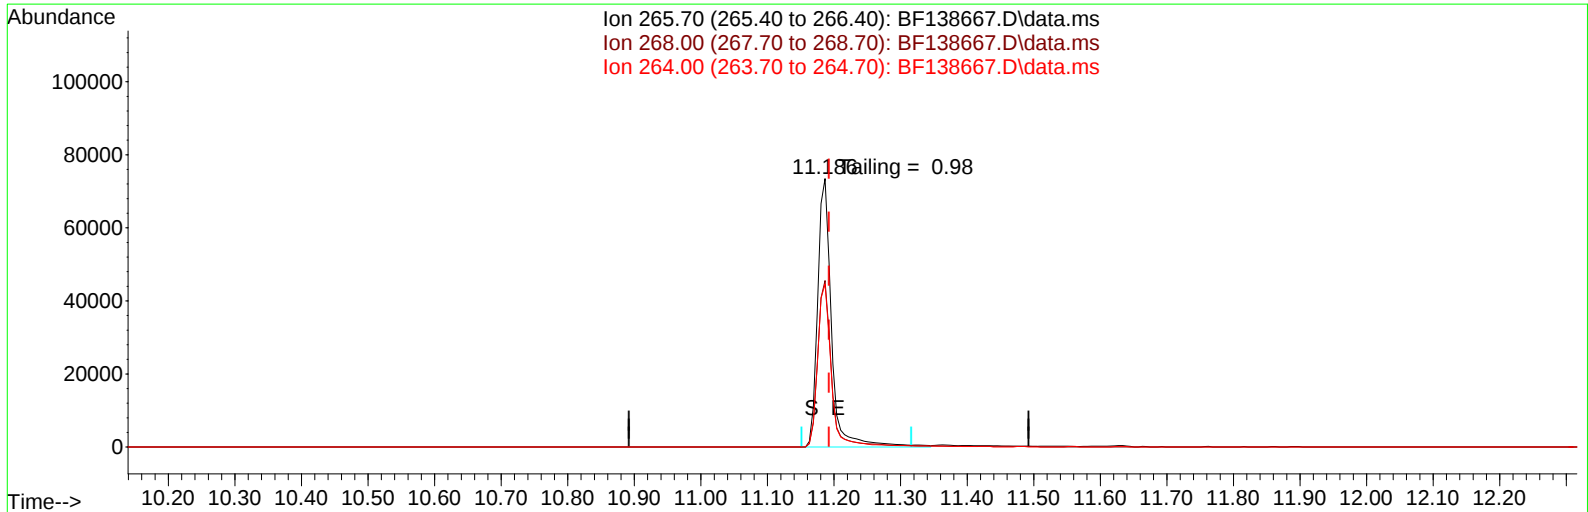

TIC: BF138667.D\data.ms

(70) Pentachlorophenol (C)

11.186min (-0.006) 24668.92 ng




response 106172

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.60	61.98
264.00	66.90	60.77
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF072924\
Data File : BF138667.D
Acq On : 29 Jul 2024 12:10
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_F
ClientSampleId :
DFTPP

Quant Time: Jul 29 13:32:14 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_F\Methods\8270-BF070924.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 09 16:58:40 2024
Response via : Initial Calibration

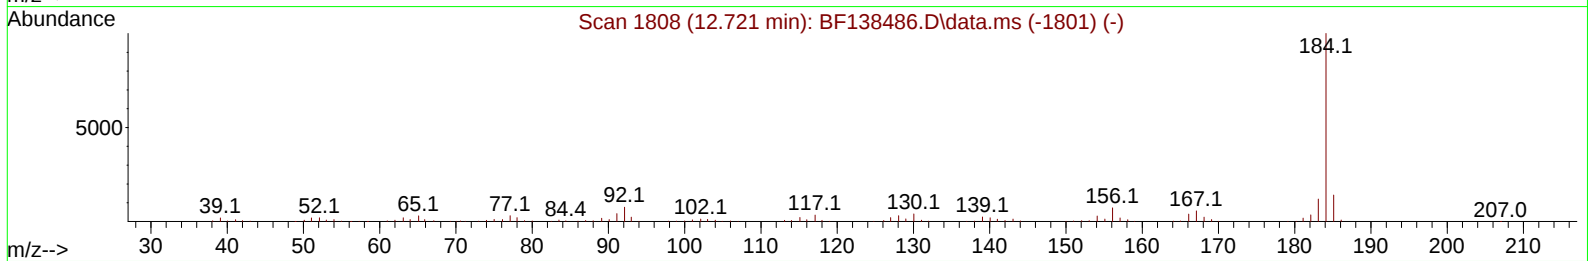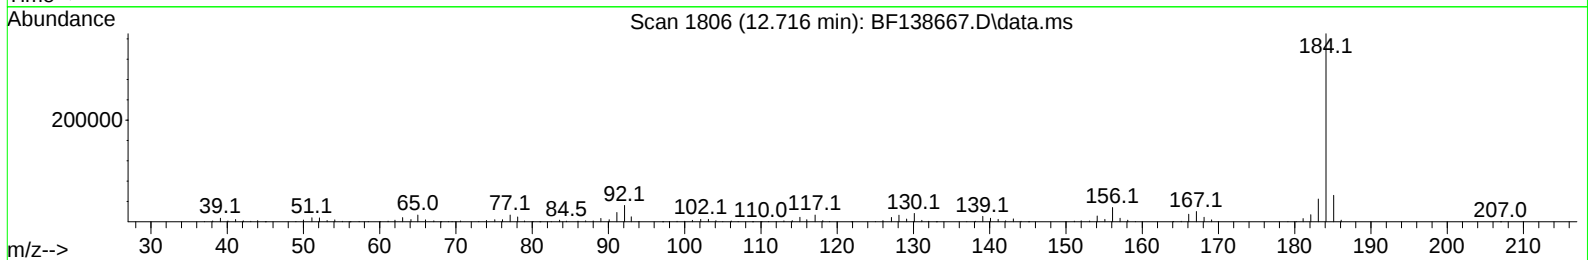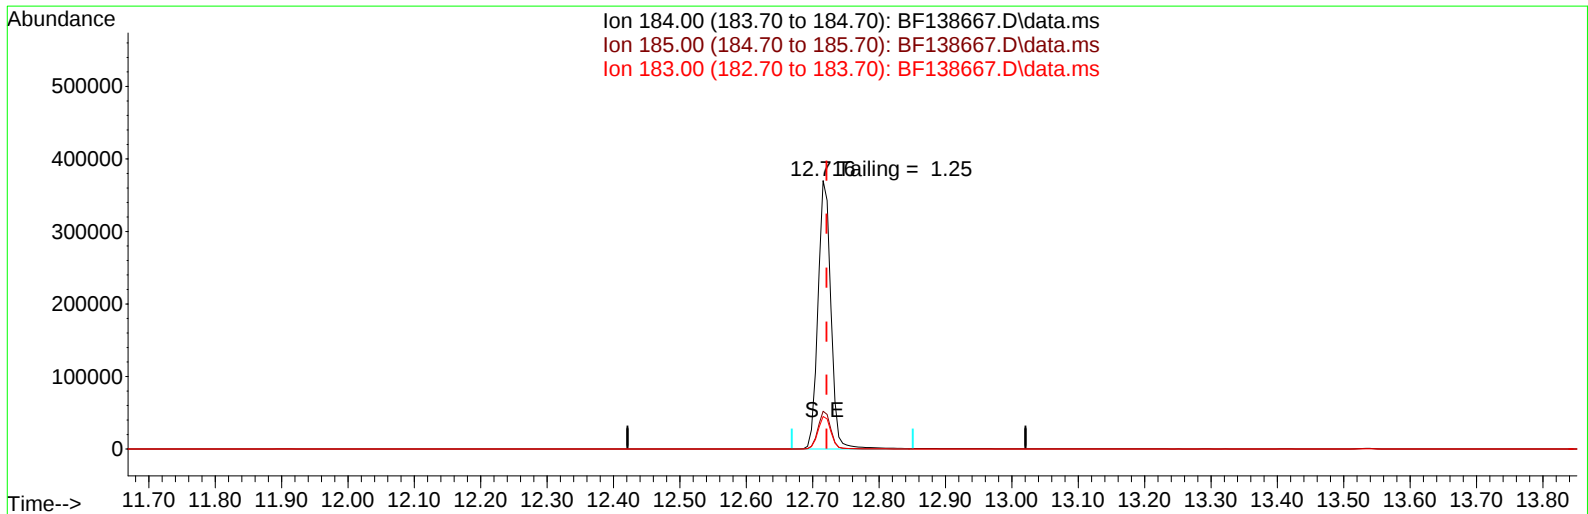

TIC: BF138667.D\data.ms

(77) Benzidine

12.716min (-0.005) 0.00 ng

response 501545

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.10	14.09
183.00	11.90	12.13
0.00	0.00	0.00