
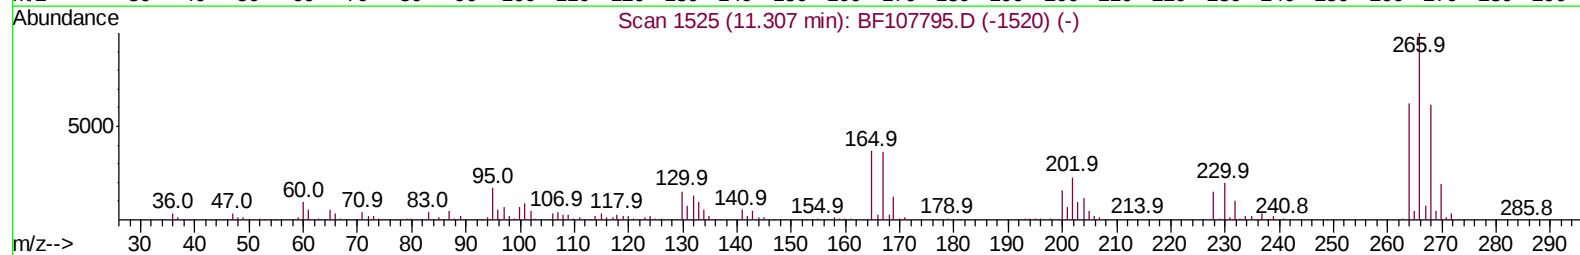
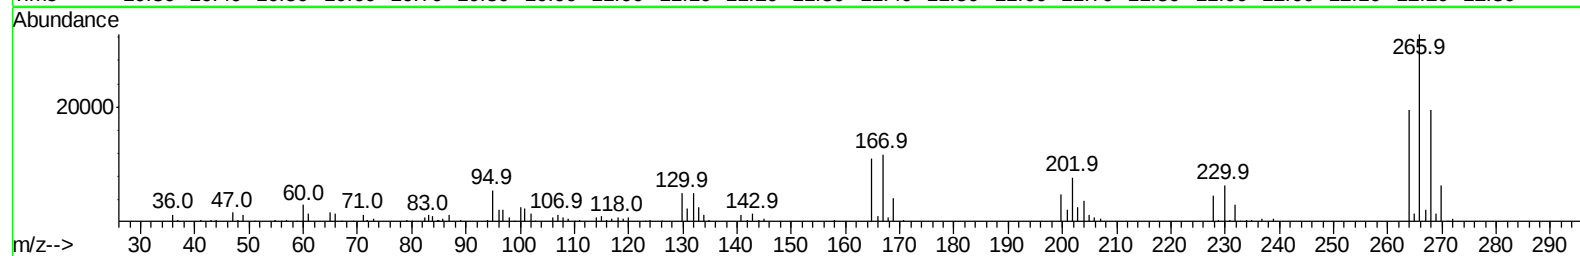


Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF073018\
Data File : BF107827.D
Acq On : 31 Jul 2018 3:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 09:23:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 30 17:48:53 2018
Response via : Initial Calibration

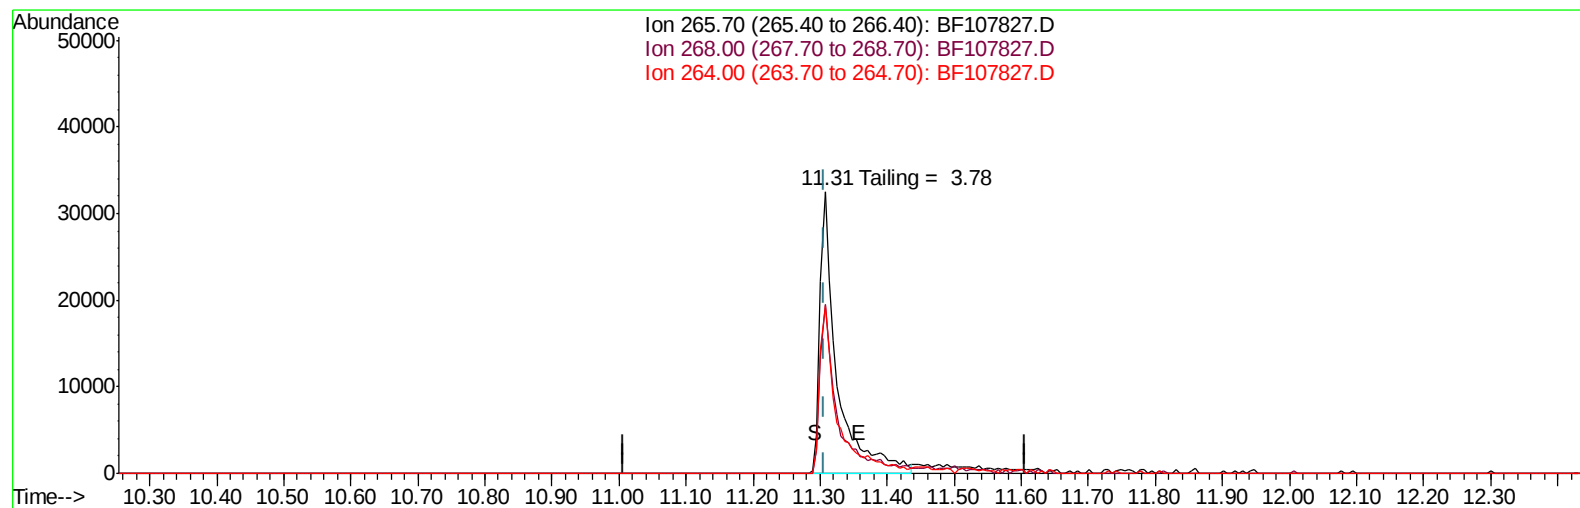

TIC: BF107827.D

(69) Pentachlorophenol (C)




11.307min (+0.000) 23992.89ng

response 56483

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	60.13
264.00	61.90	59.68
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA F\DATA\BF073018\
Data File : BF107827.D
Acq On : 31 Jul 2018 3:54
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 09:23:42 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 30 17:48:53 2018
Response via : Initial Calibration

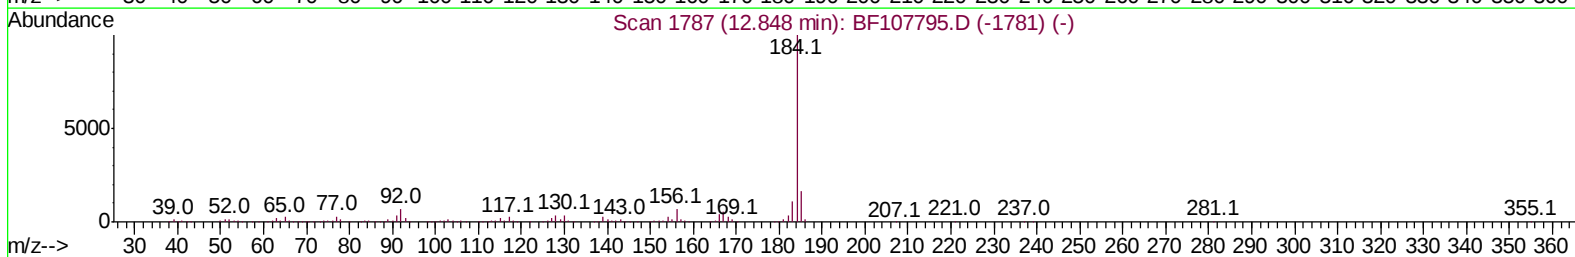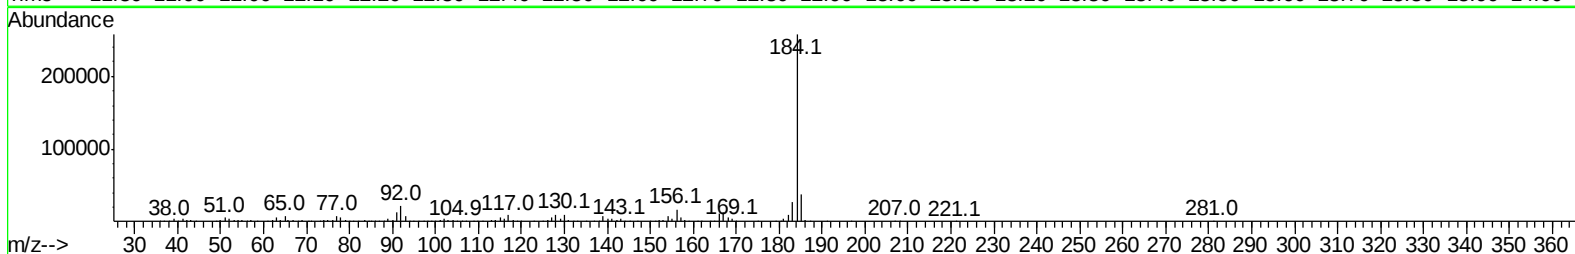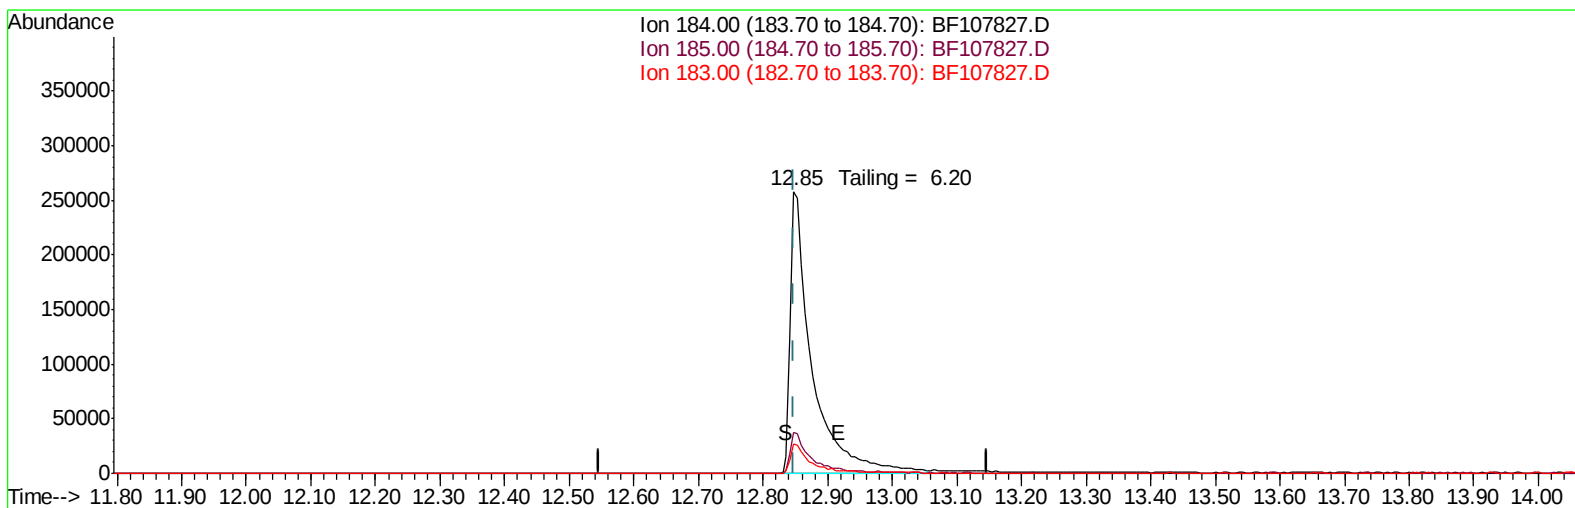

TIC: BF107827.D

(76) Benzidine

12.848min (+0.000) 62746.96ng

response 602544

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.78
183.00	11.60	10.34
0.00	0.00	0.00