


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073018\
 Data File : BF107790.D
 Acq On : 30 Jul 2018 9:50
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 30 17:48:53 2018

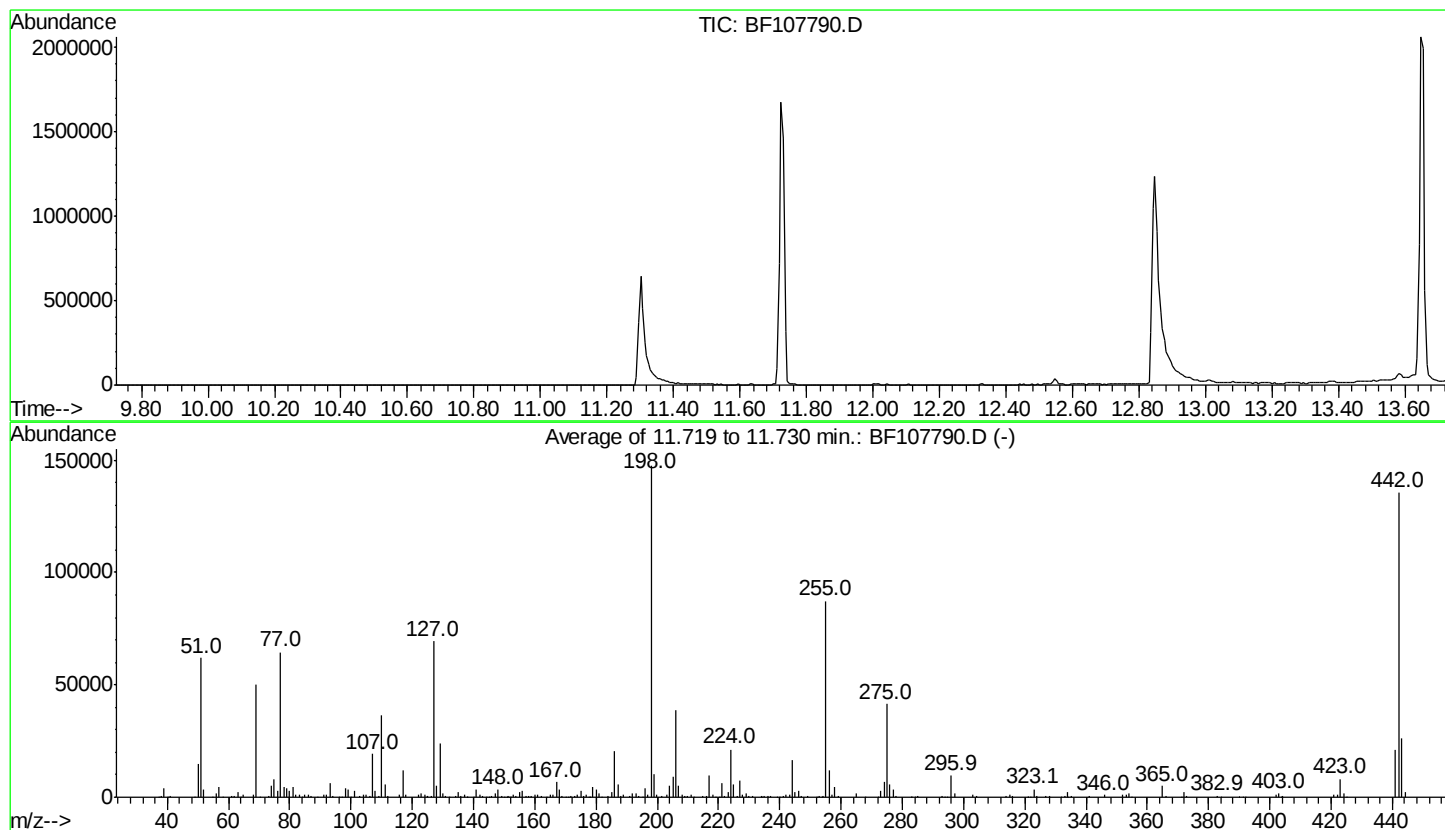

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	42.0	61912	PASS
68	69	0.00	2	2.0	1015	PASS
69	198	0.00	100	34.1	50352	PASS
70	69	0.00	2	0.3	146	PASS
127	198	10	80	47.0	69309	PASS
197	198	0.00	2	0.9	1277	PASS
198	198	100	100	100.0	147480	PASS
199	198	5	9	6.9	10219	PASS
275	198	10	60	28.0	41306	PASS
365	198	1	100	3.4	4946	PASS
441	198	0.01	100	14.2	20903	PASS
442	198	50	100	91.8	135408	PASS
443	442	15	24	19.4	26317	PASS