
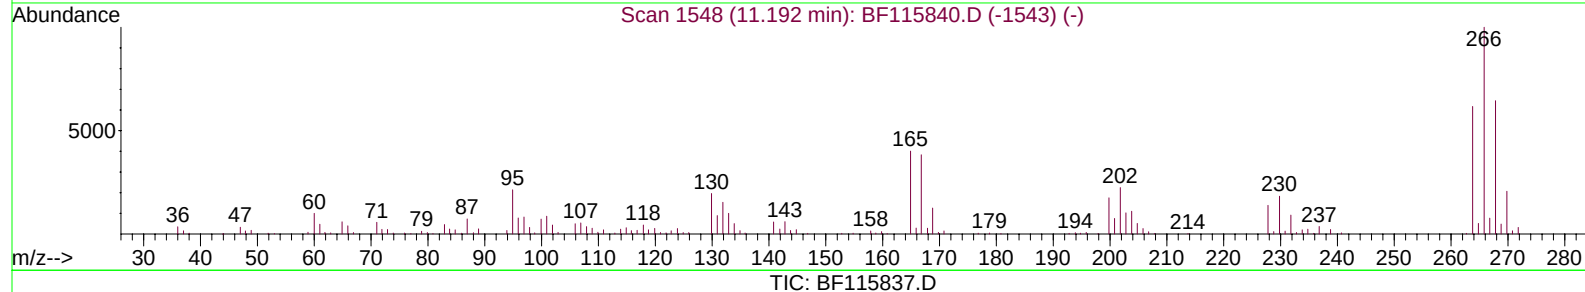
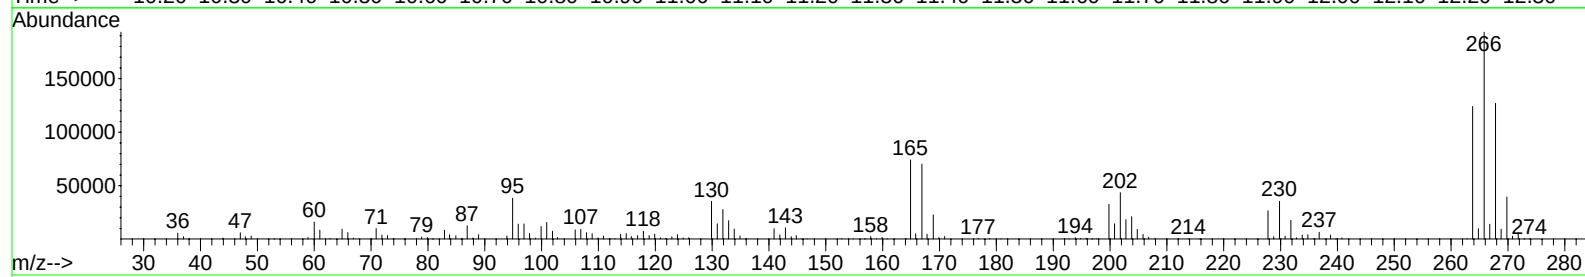


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF073019\
Data File : BF115837.D
Acq On : 30 Jul 2019 12:29
Operator : HP/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 19:11:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jul 30 16:54:32 2019
Response via : Initial Calibration

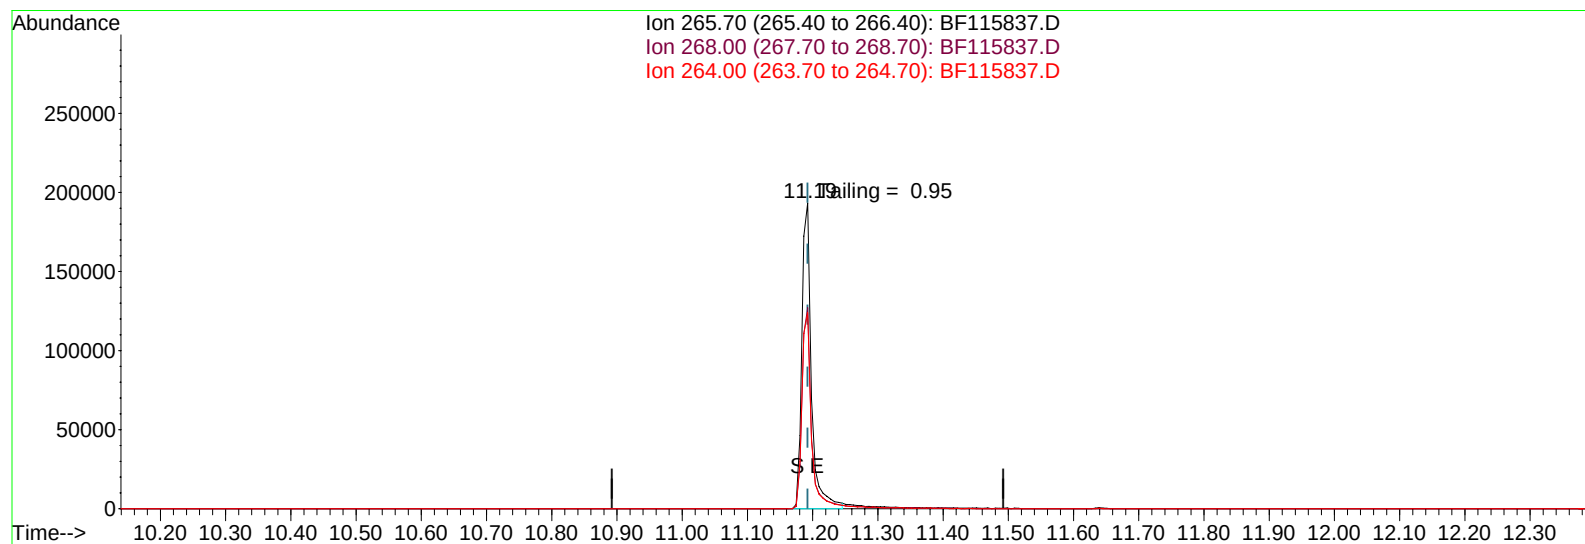

(70) Pentachlorophenol (C)




11.192min (+0.000) 145063.22ng

response 207488

Ion	Exp%	Act%
265.70	100	100
268.00	64.50	65.72
264.00	61.70	64.11
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF073019\
 Data File : BF115837.D
 Acq On : 30 Jul 2019 12:29
 Operator : HP/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 30 19:11:26 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073019.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jul 30 16:54:32 2019
 Response via : Initial Calibration

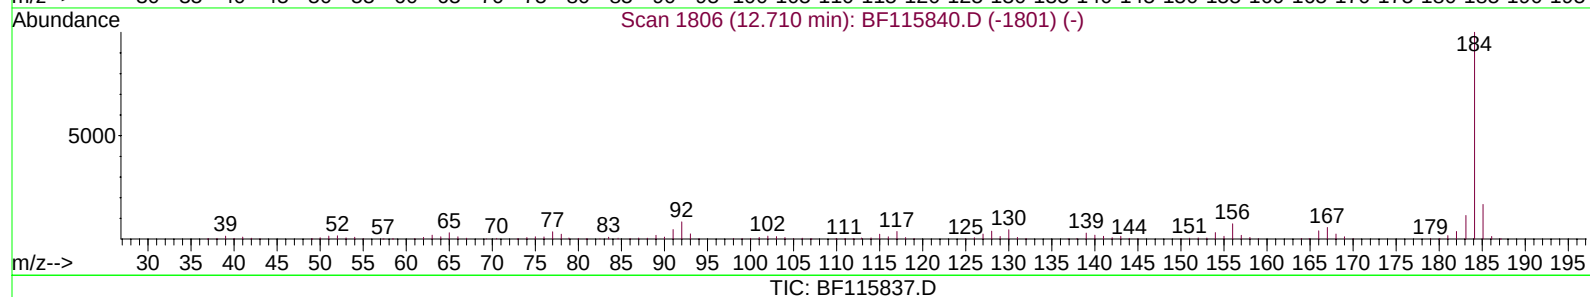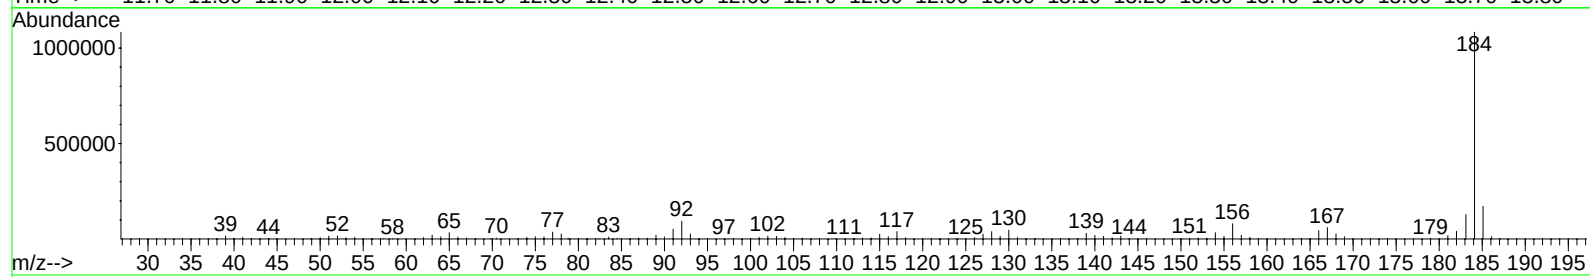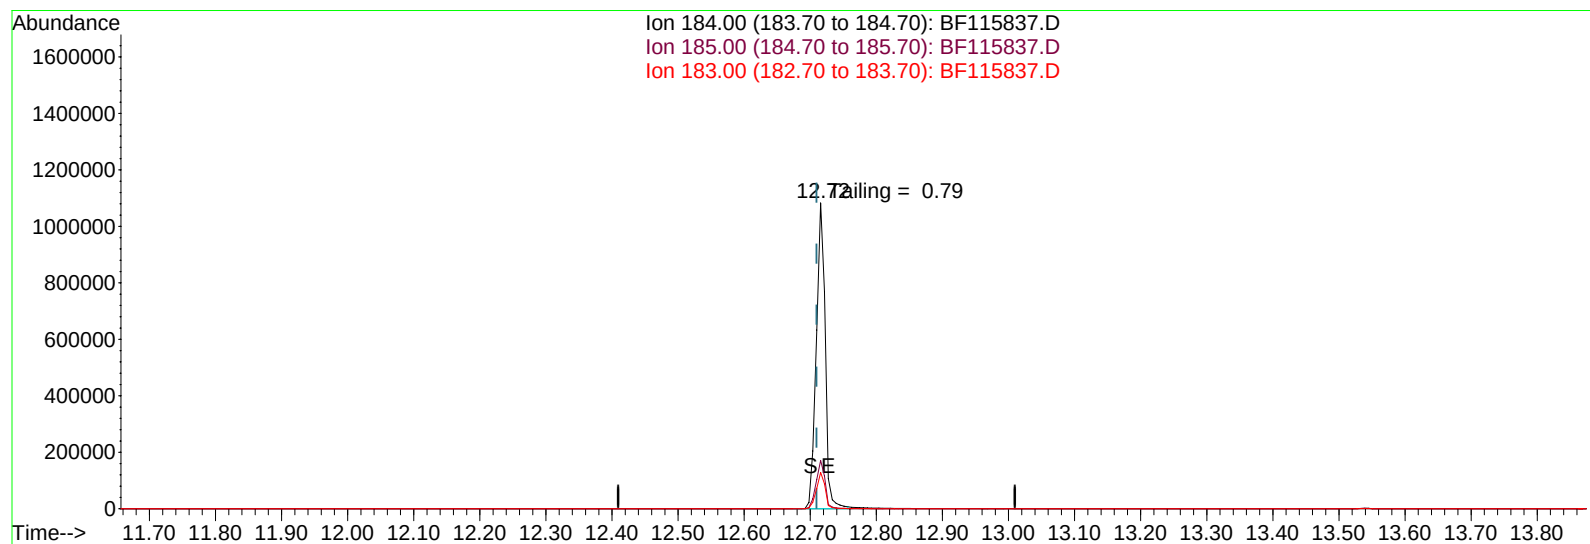

(77) Benzidine

12.716min (+0.006) 27229.30ng

response 1037670

Ion	Exp%	Act%
184.00	100	100
185.00	16.80	15.79
183.00	11.40	11.87
0.00	0.00	0.00