
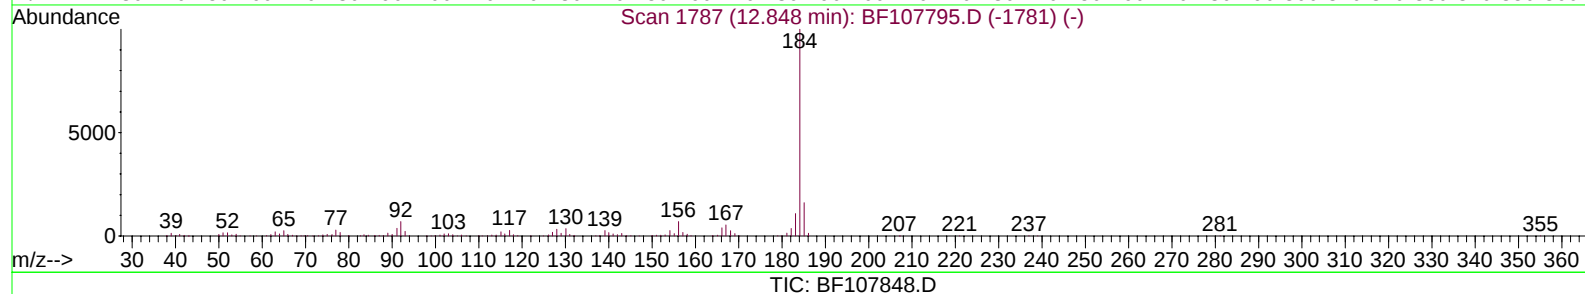
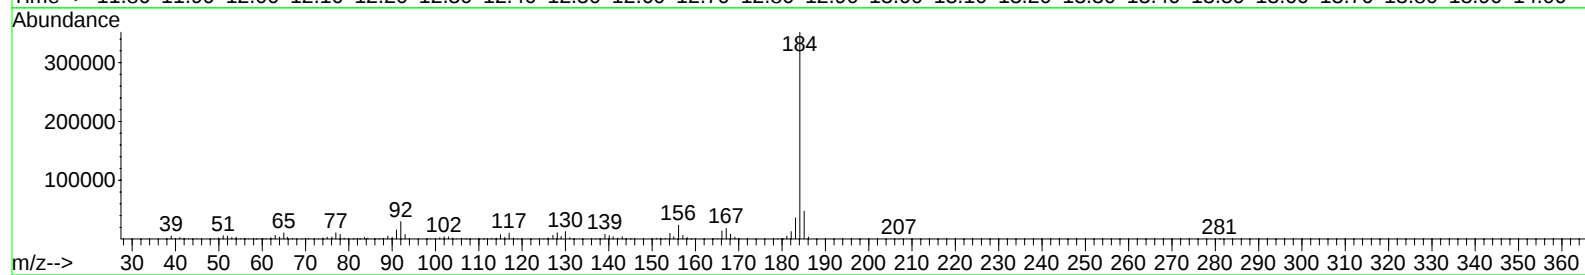


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF073118\
Data File : BF107848.D
Acq On : 31 Jul 2018 14:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 18:13:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 30 17:48:53 2018
Response via : Initial Calibration

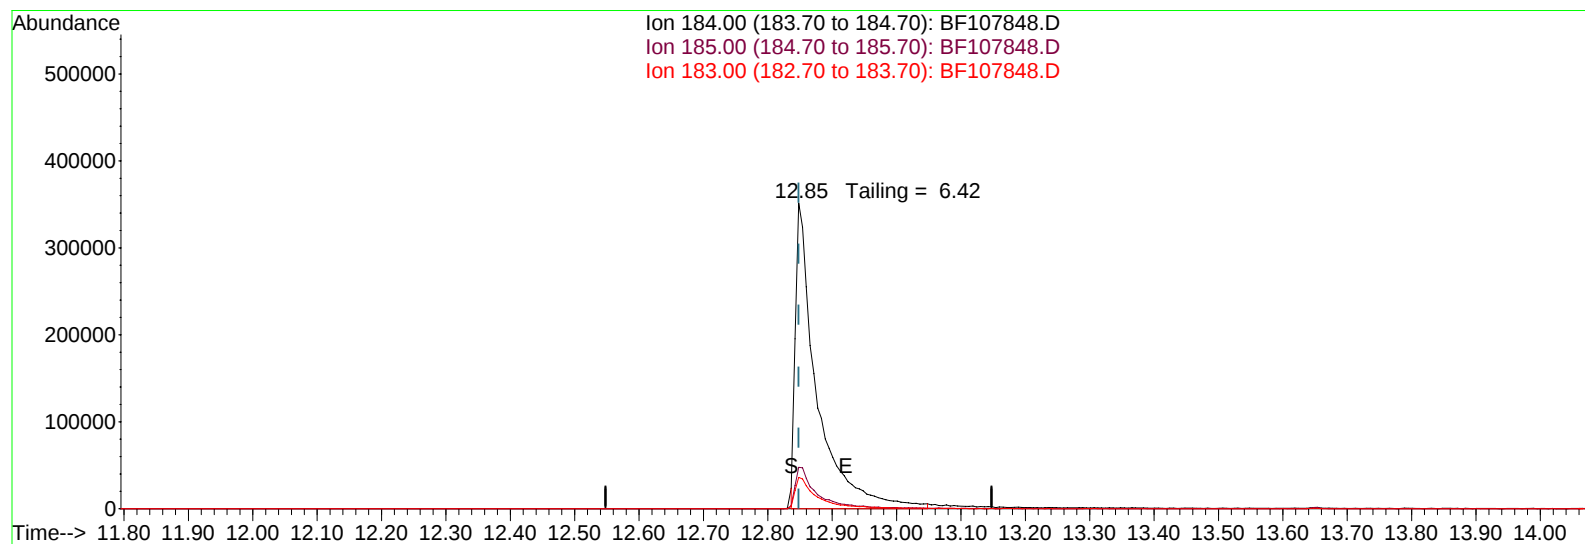

(76) Benzidine




12.848min (+0.000) 0.00ng

response 831163

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	13.55
183.00	11.60	10.28
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF073118\
Data File : BF107848.D
Acq On : 31 Jul 2018 14:41
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jul 31 18:13:54 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 30 17:48:53 2018
Response via : Initial Calibration

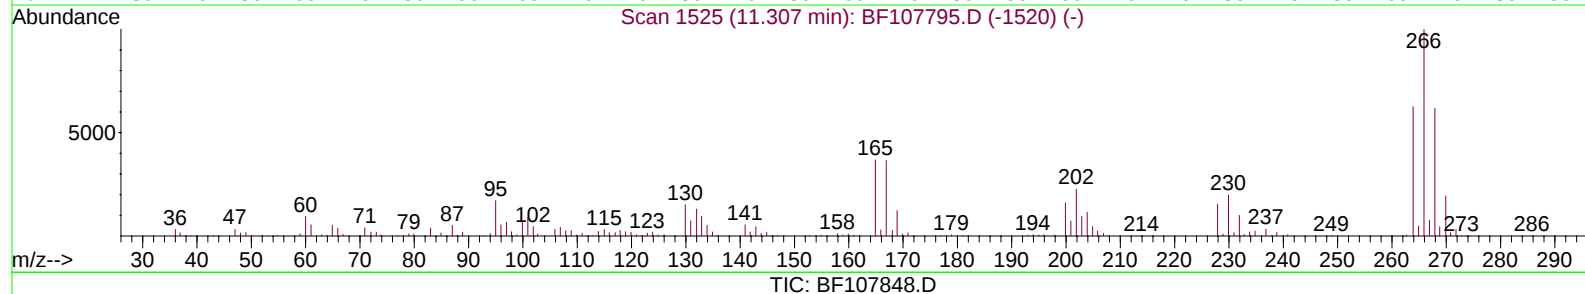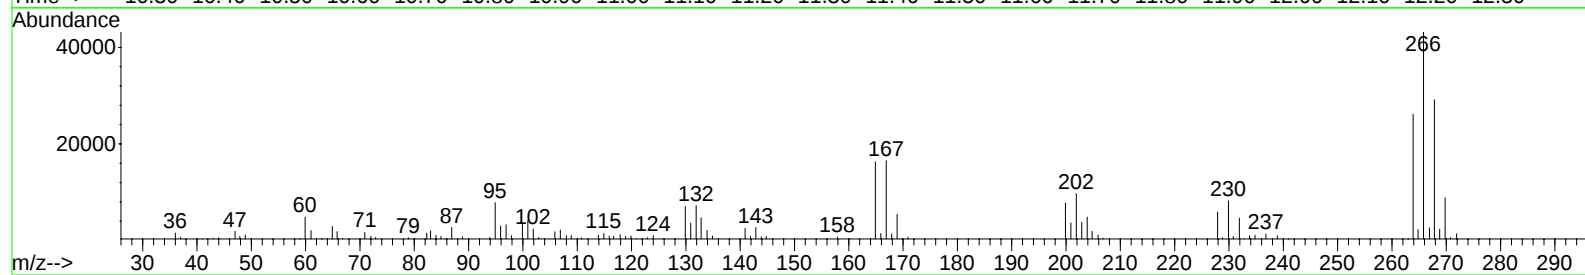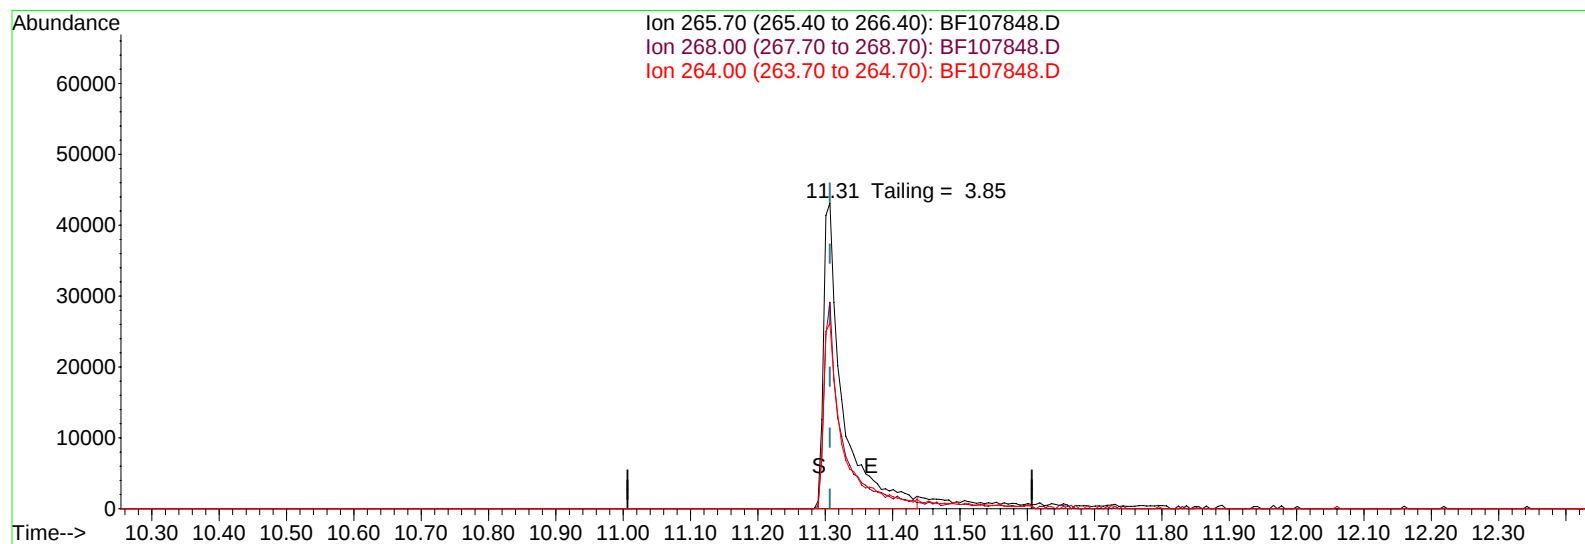

(69) Pentachlorophenol (C)

11.307min (+0.000) 21354.79ng

response 84648

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	67.56
264.00	61.90	60.65
0.00	0.00	0.00