
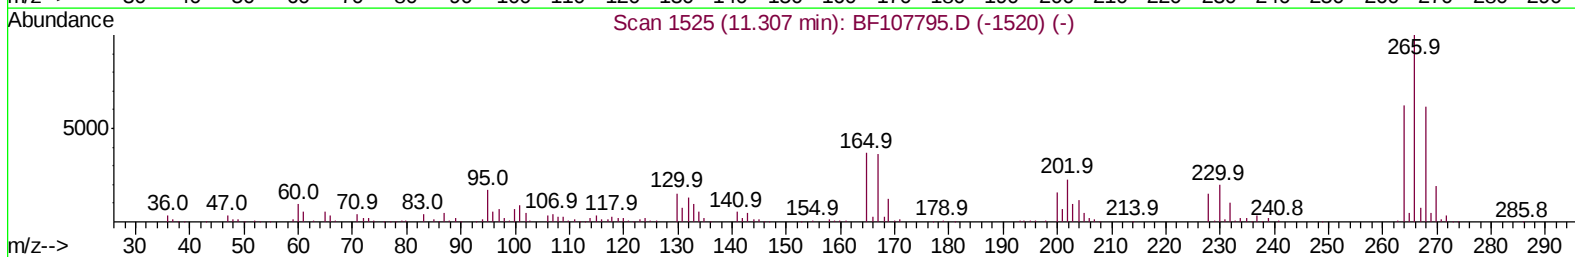
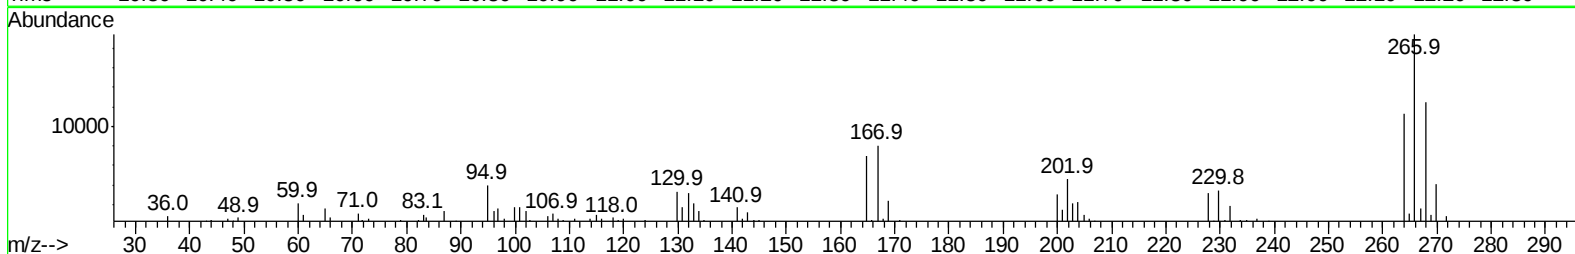


Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF073118\
Data File : BF107875.D
Acq On : 1 Aug 2018 3:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:38:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 30 17:48:53 2018
Response via : Initial Calibration

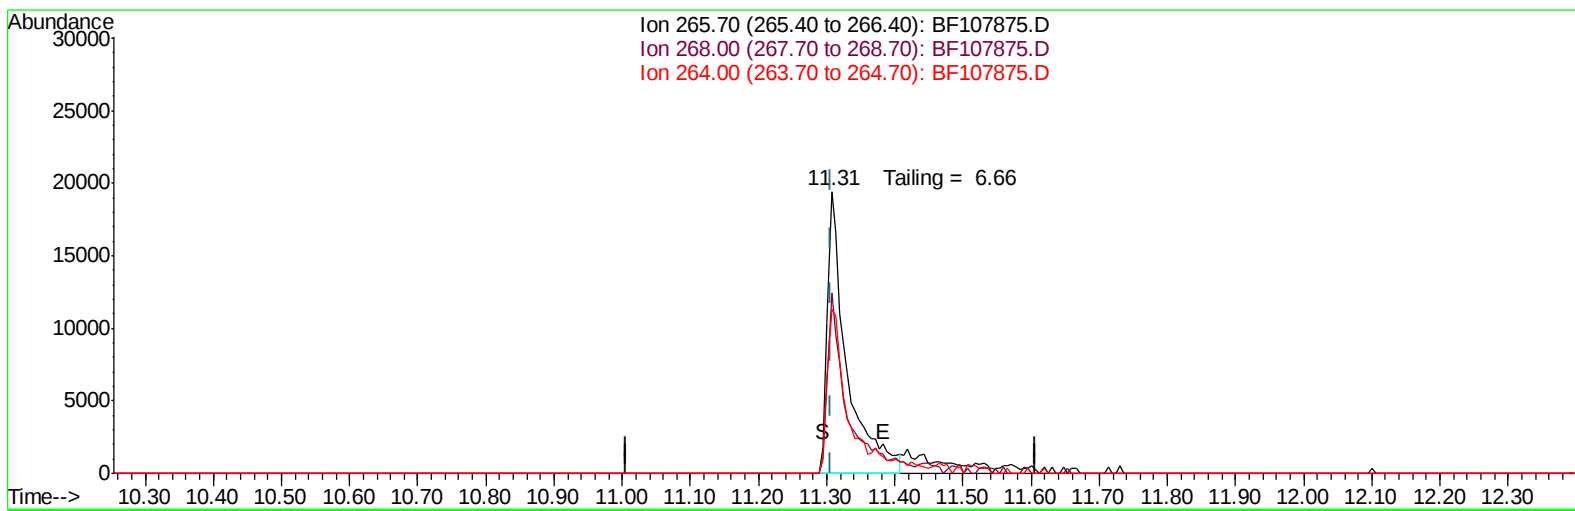

TIC: BF107875.D

(69) Pentachlorophenol (C)




11.307min (+0.000) 0.00ng

response 37481

Ion	Exp%	Act%
265.70	100	100
268.00	63.90	64.28
264.00	61.90	58.41
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA F\Data\BF073118\
Data File : BF107875.D
Acq On : 1 Aug 2018 3:15
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Aug 01 08:38:05 2018
Quant Method : Z:\SVOASRV\HPCHEM1\BNA F\METHODS\8270-BF073018.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Jul 30 17:48:53 2018
Response via : Initial Calibration

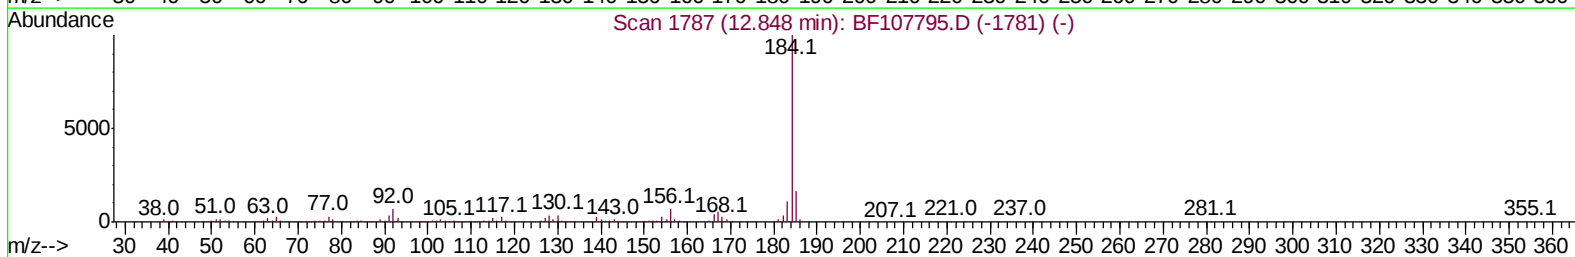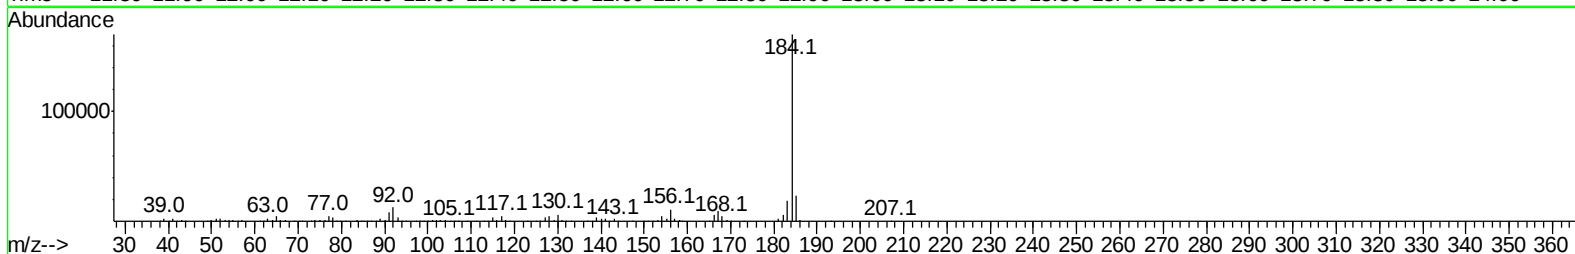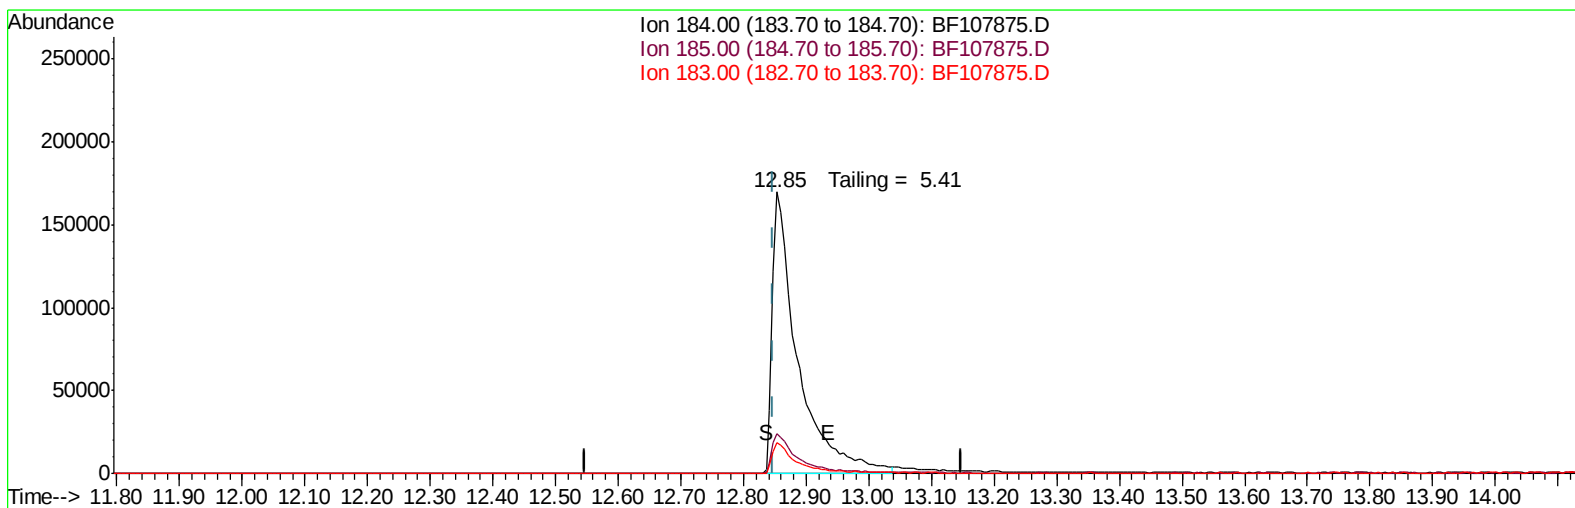

TIC: BF107875.D

(76) Benzidine

12.854min (+0.006) 15936.19ng

response 488464

Ion	Exp%	Act%
184.00	100	100
185.00	15.70	14.13
183.00	11.60	10.86
0.00	0.00	0.00