


Data Path : Z:\svoasrv\HPCHEM1\BNA_F\Data\BF073118\
 Data File : BF107848.D
 Acq On : 31 Jul 2018 14:41
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_F
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_F\METHODS\8270-BF073018.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Jul 30 17:48:53 2018

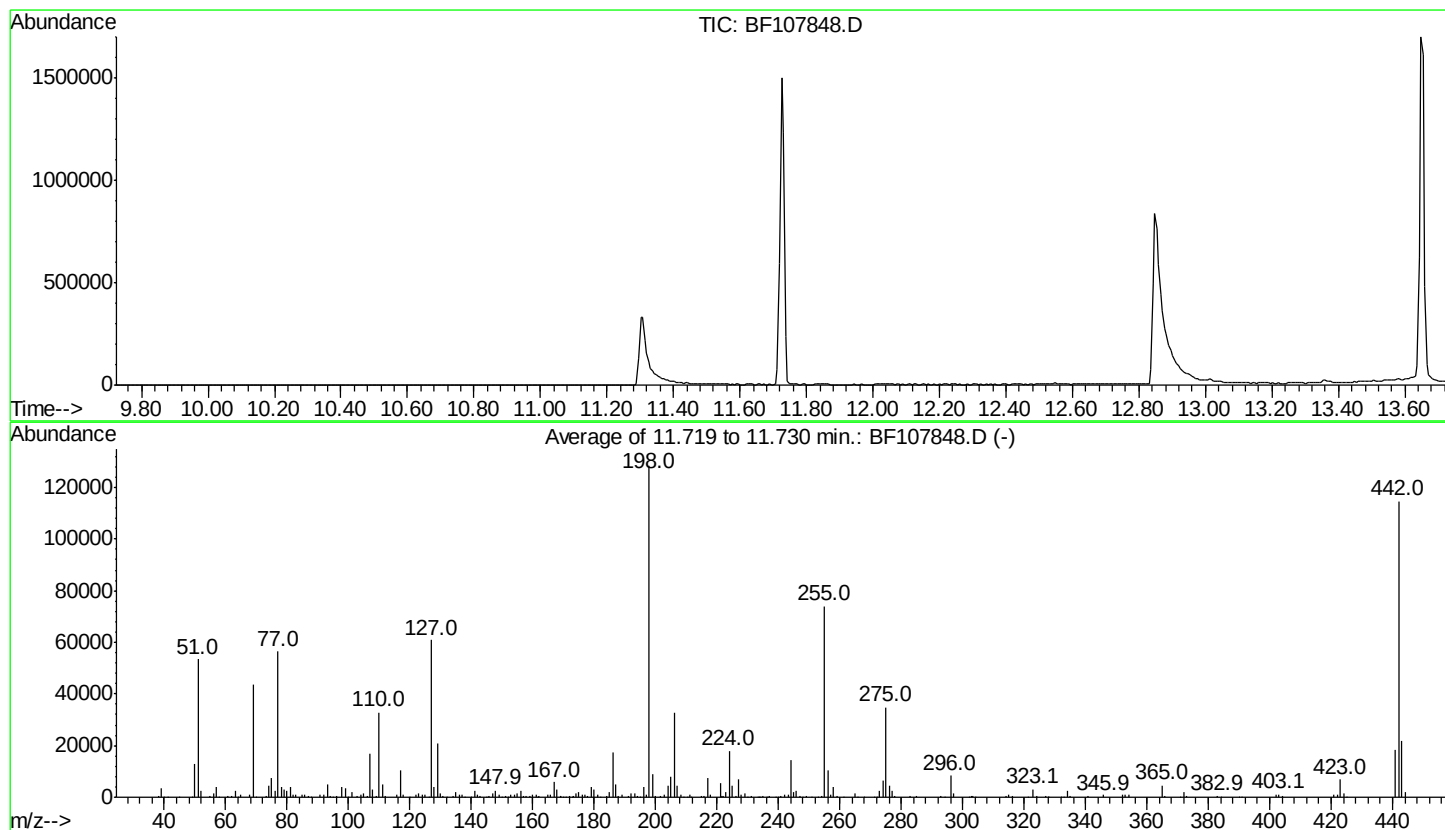

AutoFind: Scans 1595, 1596, 1597; Background Corrected with Scan 1590

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	41.5	53368	PASS
68	69	0.00	2	1.9	810	PASS
69	198	0.00	100	34.0	43733	PASS
70	69	0.00	2	0.3	127	PASS
127	198	10	80	47.3	60821	PASS
197	198	0.00	2	0.8	1081	PASS
198	198	100	100	100.0	128453	PASS
199	198	5	9	6.8	8722	PASS
275	198	10	60	27.1	34825	PASS
365	198	1	100	3.5	4487	PASS
441	198	0.01	100	14.1	18124	PASS
442	198	50	100	89.3	114733	PASS
443	442	15	24	19.2	22050	PASS